

(19)

Europäisches Patentamt
European Patent Office
Office européen des brevets



(11)

EP 0 487 110 B1

(12)

EUROPEAN PATENT SPECIFICATION

(45) Date of publication and mention
of the grant of the patent:
06.10.1999 Bulletin 1999/40

(51) Int Cl.⁶: **G06F 19/00**

(21) Application number: **91119983.4**

(22) Date of filing: **22.11.1991**

(54) Computer-aided diagnosis system for medical use

Rechnergestütztes System zur Diagnose für medizinischen Gebrauch

Système assisté par ordinateur pour le diagnostic à usage médical

(84) Designated Contracting States:
DE NL

(30) Priority: **22.11.1990 JP 32049890**

(43) Date of publication of application:
27.05.1992 Bulletin 1992/22

(73) Proprietor: **KABUSHIKI KAISHA TOSHIBA**
Kawasaki-shi, Kanagawa-ken 210-8572 (JP)

(72) Inventors:

- Yamada, Shinichi, c/o Intellectual Property Div.
Minato-ku, Tokyo 105 (JP)
- Komatsu, Kenichi, c/o Intellectual Property Div.
Minato-ku, Tokyo 105 (JP)
- Ema, Takehiro, c/o Intellectual Property Div.
Minato-ku, Tokyo 105 (JP)

(74) Representative:
Blumbach, Kramer & Partner GbR
Radeckestrasse 43
81245 München (DE)

(56) References cited:

EP-A- 0 366 076
DE-A- 3 823 251

EP-A- 0 380 966
US-A- 5 021 770

- PROCEEDINGS OF THE 12TH ANNUAL
INTERNATIONAL CONFERENCE OF THE IEEE
ENGINEERING IN MEDICINE AND BIOLOGY
SOCIETY, IEEE PRESS NEW YORK US vol. 1/5,
1 November 1990, PHILADELPHIA, US pages 219
- 220, XP000239502 YONGMIN KIM ET AL 'A
NEXT BASED HIGH PERFORMANCE IMAGE
COMPUTING WORKSTATION FOR BIOMEDICAL
APPLICATIONS'
- PROCEEDINGS OF IMAC 89, IEEE COMPUTER
SOCIETY PRESS NEW YORK US 4 June 1989,
WASHINGTON D.C., US pages 104 - 107,
XP000201387 J.H.PERRY 'PACS
WORKSTATIONS'

Best Available Copy

Note: Within nine months from the publication of the mention of the grant of the European patent, any person may give notice to the European Patent Office of opposition to the European patent granted. Notice of opposition shall be filed in a written reasoned statement. It shall not be deemed to have been filed until the opposition fee has been paid. (Art. 99(1) European Patent Convention).

EP 0 487 110 B1

Description

[0001] The present invention relates to a computer-aided diagnosis system for medical use, which outputs computer-aided diagnosis data for medical images using a computer.

[0002] Recently, a computer-aided diagnosis system (hereinafter referred to as a CAD system) for medical use has been developed in which the features of medical image data are determined and computer-aided diagnosis data (hereinafter referred to as CAD data) for assisting a doctor are obtained by using a computer. It is, however, cumbersome for a doctor to operate a computer to obtain the CAD data during the diagnosis, resulting in an adverse effect on a reading operation of image in terms of both time and labor. Further, the conventional CAD system itself cannot provide a high precision CAD data required for the diagnosis.

[0003] Examples of such CAD system are disclosed in US-A-4,851,984 and US-A-4,839,807. The CAD system described in the above US-Patents comprises means for inputting a medical image, means for analyzing the medical image using a predetermined CAD algorithm, and means for displaying an analysis result.

[0004] The doctor refers to the output of the CAD system at the time of reading of the medical image to prevent an oversight of a shadow image of the abnormal portion.

[0005] To obtain the CAD data, the following proceedings are required. Locations of one type of abnormal shadow images, e.g., an abnormal shadow image of the interstitial lung disease, are detected on a conventional X-ray radiograph and the result of the detection is output. Therefore, the medical image on the X-ray film is digitized. A rib, an object of the analysis, is identified in the medical image. A region of interest (hereinafter referred to as a ROI) is set on the medical image, as described in the US-A-4,851,984. The data in the ROI is frequency-analyzed to extract the amount of physical texture of the image. The shadow image is classified into groups based on the amount of physical texture. A display device displays the digital image and the type, degree, and position of the shadow image in an overlapping manner.

[0006] The reading operation by the doctor is to draft the reading report. Before drafting the report, the doctor refers to the CAD data to prevent an oversight of a shadow image.

[0007] If the doctor needs the CAD data, the above proceedings must be performed. That is, the medical image must be digitized before the CAD system starts to operate. The digitized image is analyzed by the computer using the above proceedings and the analysis result is output to an attached display device. The doctor continues the reading of the image after watching the CAD result.

[0008] The above described CAD system has following drawbacks.

[0009] The same CAD algorithm which is included in the CAD system is applied to the image data regardless of the type of the image. For example, the same CAD algorithm is applied to a conventional X-ray radiograph of chest as well as a CT image. Therefore, an unexpected CAD result is obtained thus lowering the ability of diagnosis.

[0010] The CAD system includes only one CAD algorithm for a given disease. Therefore, it is not possible to obtain a plurality of CAD data for a plurality of diseases. Therefore, if ten diseases are to be detected from one image based on the CAD data, the image data must be input to ten CAD systems and ten CAD data must be output. This increases the time and labor for the CAD operation.

[0011] A time for merely reading the image without outputting the CAD data is about three minutes. A time from requesting a kind of CAD operation to output the CAD data is about two minutes. If the CAD operation is performed during the reading, it takes a long time for reading and a difficulty occurs for the reading.

[0012] The CAD data includes many items, e.g., the position, type, and degree of the abnormality. In the conventional CAD system, all the items of data are output, thereby the output becomes complicate.

[0013] The CAD system does not store the CAD result, therefore, if the CAD operation is requested for the image which has been once analyzed, the same CAD operation is repeated thus wasting the time.

[0014] Meanwhile, a picture archiving communication system (hereinafter referred to as a PACS) for transferring, storing, and displaying the medical images has been developed. In the PACS, digital medical image data archived by modalities including a digitizer and attribute data thereof are transferred via a network and are stored in a large capacity recording means such as an optical disk device. Desired data are retrieved by using a data base system. The image data is transferred to a workstation via the network and is displayed. However, the prior PACS does not perform a CAD operation.

[0015] EP-A-0 366 076 discloses a PACS system wherein image data and image addition data are stored in a data base. The PACS comprises medical diagnosis apparatuses which are coupled to work stations via interface units and a star coupler. The system generates an unread examination list and a read examination list which are transferred to the work stations at the time of a reading operation wherein the list data of the read examination list is arranged in accordance with a desired priority order.

[0016] Shimadzu Review, Japan, July 1990, Vol. 47, No. 2, pages 163 to 168; M. Andoh et al: "Shimadzu AI-PACS SAIPACS" discloses a PACS system wherein the work stations are arranged to perform a computer-aided diagnosis and a computer-aided diagnostic reporting, by using artificial intelligence technique.

[0017] It is an object of the present invention to provide a system for analyzing a medical image using a

computer-aided diagnosis algorithm, for medical use, which outputs computer-aided diagnosis data with high precision by a simple operation having no adverse effect on diagnosis made by doctors.

[0018] This object is achieved by the features mentioned in independent claim 1.

[0019] Some preferred implementations are defined in the subclaims.

[0020] The present invention thus also provides a picture archiving communication system incorporating the computer-aided diagnosis system for medical use and having a high diagnosis precision.

[0021] This invention can be more fully understood from the following detailed description when taken in conjunction with the accompanying drawings, in which:

Fig. 1 is a block diagram showing the arrangement of a first embodiment of a computer-aided diagnosis system for medical use according to the present invention;

Fig. 2 shows items of examination data;

Fig. 3 shows a practical example of the examination data for a conventional X-ray radiograph of chest;

Fig. 4 is a block diagram showing the arrangement of a film digitizer shown in Fig. 1;

Fig. 5 shows items of relevant data;

Fig. 6 shows a practical example of the relevant data;

Fig. 7 is a view for defining an imaging direction in the conventional X-ray radiography;

Fig. 8 is a block diagram showing the arrangement of a data base shown in Fig. 1;

Fig. 9 shows an examination directory included in a data retrieving device shown in Fig. 8;

Fig. 10 shows the relationship between a doctor ID and a requesting doctor ID which is used when the image is transferred to a workstation at the time of reading;

Fig. 11 shows an operation for transferring the images which has been examined to the workstation at the time of reading;

Fig. 12 is a block diagram showing the arrangement of the workstation shown in Fig. 1;

Fig. 13 shows an example of the images displayed on the workstation in the PACS at the time of diagnosis of the conventional X-ray radiograph;

Fig. 14 shows a CRT image display control table for managing the display of the workstation;

Fig. 15 shows a table registering the relationship between the name of a CAD algorithm and associated attribute data of the image which is applied with the CAD algorithm;

Fig. 16 is a view showing a practical example of ROI setting in lungs;

Fig. 17 is a block diagram schematically showing an algorithm for automatically setting an ROI;

Fig. 18 is a detailed block diagram for explaining the diagram of Fig. 16;

Fig. 19 is a block diagram schematically showing an algorithm for obtaining the amount of textures in the ROI;

Fig. 20 is a flow chart schematically showing an algorithm for determining based on the amount of textures whether the ROI is normal or abnormal;

Fig. 21 is a block diagram performing the operation shown in Fig. 20;

Fig. 22 shows an example of the data format of a CAD result;

Fig. 23 is a view showing a practical example of the CAD result data;

Fig. 24 is a perspective view showing a touch panel as an example of an input device of the workstation;

Fig. 25 is a view showing a display example of the touch panel;

Fig. 26 is a view for explaining an example of a schematic naming of abnormal positions;

Fig. 27 shows a relationship between locations and coordinates of the abnormal positions;

Fig. 28 shows a table for explaining an example of detailed naming of the abnormal positions;

Fig. 29 shows an example of a text sentence display;

Fig. 30 shows an example of marker display;

Fig. 31 shows an example of detailed CAD display using the marker shown in Fig. 30;

Fig. 32 shows another example of the marker display;

Fig. 33 shows an ROC curve display as an optional CAD output;

Fig. 34 shows the data format of a CAD result;

Fig. 35 shows a practical example of the CAD result;

Fig. 36 is a block diagram showing the arrangement of a CAD processor included in a second embodiment of a computer-aided diagnosis system for medical use according to the present invention;

Fig. 37 is a block diagram showing the arrangement of a sound output device as a main part of a third embodiment of the present invention;

Figs. 38A and 38B show examples of a menu window display according to a seventh embodiment of the present invention;

Fig. 39 is a block diagram showing the arrangement of a computer-aided diagnosis system according to an eleventh embodiment of the present invention;

Figs. 40A to 40E show modifications of marker display according to a twelfth embodiment;

Figs. 41A to 41F show other modifications of the marker display according to the twelfth embodiment;

Figs. 42A and 42B show still another modifications of the marker display according to the twelfth embodiment; and

Fig. 43 shows an example of a table formed of names of algorithms stored in a memory in a seventeenth embodiment of the present invention.

[0022] A preferred embodiment of a computer-aided diagnosis system for medical use according to the present invention will now be described with reference to the accompanying drawings. Though it is possible to embody the CAD system as a stand-alone system, an embodiment of the CAD system incorporated into the PACS will be described. Fig. 1 is a block diagram showing the first embodiment constructed on the basis of the PACS. In general, the PACS is a system for performing storage and transferring of various types of digital image data produced in a single or a plurality of hospitals, and is formed of an image data source 10 (hereinafter referred to as a modality), a data base 12, a workstation 14 as a display unit, and a network 16 for connecting these components.

[0023] The modality 10 includes various diagnosis devices for generating medical digital images, such as a film digitizer 18 for digitizing an image of an X-ray film obtained by an X-ray radiography apparatus, an angiography imaging apparatus 20, a computed tomography (CT) scanner 22, a magnetic resonance imaging (MRI) system 24, a nuclear medicine diagnosis apparatus 26, an ultrasound diagnosis apparatus 28, and an electric endoscope 30.

[0024] An examination ordering system 32 is also connected to the network 16 via a gateway 34. The examination ordering system 32 supplies examination data indicating details of examination on individual patients to the network 16. In this manner, the PACS performs control of data on the basis of correspondence between image data obtained by examination by the modality 10 and attribute data (including examination data, relevant data, and amend and/or update data for these data supplied from the workstation 14 and the data base 12). It is noted that the number of each of the modalities 10, the data base 2, and the workstation 14 is not limited to that of the above arrangement but can be increased or decreased as needed.

[0025] Fig. 2 shows an example of items of examination data input by the examination ordering system 32 and supplied to the network 16. An examination ID number is issued every time examination is performed. In the examination ordering system 32, such examination data is input by a doctor or a person in charge at the start of examination, and a technician of the modality executes examination on a patient upon receiving the examination request, thus obtaining image data. Each frame of the image data is associated with the relevant data. An example of the relevant data is shown in Fig. 5.

[0026] When, for example, radiographic examination using a conventional X-ray radiography apparatus is necessary, examination data as shown in Fig. 3 is input from the examination ordering system 32. A radiographic technician of the conventional X-ray radiography apparatus (not shown) takes conventional X-ray radiographs according to the input examination data. In the case of a conventional X-ray radiograph, digital image data can be obtained by digitizing the image of the X-

ray film by the film digitizer 18. The image data, for example, consists of an array of data obtained by dividing the X-ray film into a matrix of $1,024 \times 1,024$ pixels and representing the density of each pixel by a digital number of 10-bit.

[0027] Fig. 4 shows the arrangement of the film digitizer 18. The film digitizer 18 comprises a controller 40, an input device 42, a display device 43, a read-only memory (ROM) 44, an examination/relevant data storing device 46, an image data storing device 48, a semiconductor memory 50, a film density detector 52, a central processing unit (CPU) 54, and a network interface (I/F) 56. Of these components, the controller 40, the input device 42, the display device 43, the ROM 44, the examination/relevant data storing device 46, the image data storing device 48, the semiconductor memory 50, the film density detector 52, the CPU 54, and the network I/F 56 are connected to a control bus line 58. The ROM 44, the image data storing device 48, the semiconductor memory 50, the film density detector 52, and the network I/F 56 are connected to an image bus line 60. The network I/F 56 is connected to the network 16.

[0028] The film density detector 52 divides an X-ray radiograph into a matrix of $1,024 \times 1,024$ pixels. The density detector 52 scans each pixel with a laser beam and measures the intensity of transmitted light to obtain the density of the pixel, thereby forming an intensity distribution of the transmitted light of the X-ray radiograph. This intensity distribution is converted into digital intensity data, and the data is supplied to the data storing device 48 through the image bus 60 and is stored therein as the image data. At the same time, examination data, together with relevant data, is stored in the examination/relevant data storing device 46. At this time, the display device 43 displays a prompt message for urging a technician to input an imaging direction of radiograph if the imaging direction is not input. When the text character denoting the imaging direction is input from the input device 42 such as a keyboard, this data is written in the column of the imaging direction of relevant data (Fig. 5) stored in the storing device 46.

[0029] Fig. 6 shows a practical example of the relevant data. The imaging direction of radiograph is defined, as shown in Fig. 7, such that when X-rays radiated from the back of a patient are detected on an X-ray film placed in front of the patient, the resulting image is referred to as a front image. Similarly, a right-side (left-side) image is defined as an image obtained when X-rays radiated from the left (right) side of the patient are detected on a X-ray film placed on the right (left) side of the patient. When digitizing of one frame of the X-ray radiograph is completed, the image data and the corresponding relevant data are associated with each other by means of the image ID number. The examination data and the corresponding relevant data are associated with each other by means of the examination ID number. The image data, the corresponding examination data, and the corresponding relevant data are supplied to the

network 16 via the network I/F 56 and transferred to the data base 12 or the workstation 14 as data flowing through the network 16.

[0030] Fig. 8 shows the arrangement of the data base 12. The data base 12 comprises a CPU 62, a ROM 64, a semiconductor memory 66, a controller 68, a data retrieving device (including an examination directory) 70, a data compression circuit 71, an image data storing device 72, and a network interface (I/F) 74. Of these components, the CPU 62, the ROM 64, the semiconductor memory 66, the controller 68, the data retrieving device 70, the data compression circuit 71, the image data storing device 72, and the network I/F 74 are connected to a control bus line 76. The ROM 64, the semiconductor memory 66, the data compression circuit 71, the image data storing device 72, and the network I/F 74 are connected to an image bus line 78. The network I/F 74 is connected to the network 16.

[0031] The image data, the corresponding examination data, and the corresponding relevant data, which are flowing through the network 16, are input to the data base 12 via the network I/F 74, and stored in the image data storing device 72. If necessary, these data, particularly the image data is temporarily stored in the semiconductor memory 66 as a buffer memory. In this case, after the amount of the data is compressed to 1/2 or 1/10 by the data compression circuit 71, the data is stored in the image data storing device 72. The examination data and the relevant data are registered in the examination directory of the data retrieving device 70 to retrieve desired examination data and relevant data using an examination ID and read out items of data.

[0032] Fig. 9 shows an example of data contained in the examination directory of the data retrieving device 70 of the data base 12. Referring to Fig. 9, reference symbol N denotes the number of images obtained in one examination. The examination directory is formed of examination data (Fig. 2), address data for storing the reading report, amount of data of the reading report, and N number of image data included in the examination. Each of the image data is formed of address data for storing the relevant data, amount of data of the relevant data, address data for storing the image data, amount of image data, and first CAD result to n-th CAD result. The CAD result is formed of a CAD ID number and address data for storing the CAD result.

[0033] Next, an image reading operation performed by a doctor for the digital images whose attribute data are stored in the data base 12 as described above will be described. In hospitals, the image reading is performed to obtain a diagnosis result from medical images. The image reading in the PACS is that images are displayed on a display device such as a CRT of the workstation 14 and a doctor makes a diagnosis from the displayed images or X-ray film obtained in the conventional X-ray radiography examination.

[0034] When a doctor for image reading inputs his or her ID number with the power source of the workstation

14 ON, the workstation 14 is set ready for receiving an image reading request. This is the same procedure as the log in operation in the conventional computer system. At this time, the workstation 14 sends a transfer request for images of a patient as an object to be image-read to the data base 12 on the basis of the examination ID input by the doctor or the examination ID which is registered in association with the doctor ID as shown in Fig. 10. If the patient has been examined, the workstation 14 may send a transfer request for images which have been read or viewed but are necessary to be referred as well as images which is not read or viewed. The necessary images are retrieved by means of, for example, the data base 12. All the examination IDs relating to the patient ID and the necessary image data are determined using a logical procedure, for example, as shown in Fig. 11. The examination IDs having the same patient and the same modality are retrieved to make a list of the examination IDs. Alternately, the examination IDs having the same patient and the same object are retrieved to make a list of the examination IDs. The examination IDs in one of the above two lists which has a high priority are sorted in the reverse chronological order.

[0035] The data base 12 selects images in units of examinations to be transferred by using the examination ID as a retrieval key. The selected image data in units of examinations or the compressed image data if the data is read out from the storing device 72, the relevant data, and the examination data in units of examinations are transferred to the network 16 via the network interface 74, and in turn to the workstation 14 sequentially.

[0036] A section for performing a CAD will be described below. The CAD is to obtain CAD data, for example, denoting a position of an abnormality in the image, by processing image data using a computer. In this embodiment, for example, the workstation 14 serves as a section for obtaining the CAD data.

[0037] Fig. 12 shows the arrangement of the workstation 14. The workstation 14 comprises an input device 80, an output device 82, an alarm generator 83, a hard disk interface (HD I/F) 84, a semiconductor memory 86, a CPU 88, a timer 90, a ROM 92, a network interface (LAN I/F) 94, a plurality of image memories 100, a plurality of CRT displays 102, a hard disk unit (HD) 106, and a data expansion circuit 108. Of these components, the input device 80, the output device 82, the alarm generator 83, the HD I/F 84, the semiconductor memory 86, the CPU 88, the timer 90, the ROM 92, the LAN I/F 94, and the data expansion circuit 108 are connected to a control bus line 96. The output device 82, the alarm generator 83, the HD I/F 84, the semiconductor memory 86, the ROM 92, and the LAN I/F 94 are connected to a high speed bus line 98. The LAN I/F 94 is connected to the network 16.

[0038] The image memories 100 are provided in one-to-one correspondence with one or more (in this case, four) CRT displays 102. Each of the image memories

100 has two or three overlay screens (plane memories) and is connected to the output device 82. An output from the image memory 100 is displayed on the corresponding CRT display 102. The HD unit 106 is connected to the HD I/F 84. In the workstation 14, the image data input via the LAN I/F 94 in the form of the compressed image data, the corresponding relevant data, and the examination data in units of examinations are stored in the HD unit 106.

[0039] In order to perform an image reading, a doctor selects an image and the attribute data and the image is displayed on the CRT display 102 via the output device 82. The image to be displayed is selected among the images for one examination using the image ID input by the doctor. If the compressed image data is read out from the HD unit 106, the compressed data is expanded by the data expansion circuit 108 and then stored in the semiconductor memory 86. The relevant data and the examination data are also stored in the semiconductor memory 86. The image data is read out from the semiconductor memory 86 and is displayed on the CRT display 102 to be read or viewed by the doctor. For example, when an object to be image-read is a conventional X-ray radiograph, front and side images are usually displayed. When the patient has been examined, both non-read and past images (other than the non-read image; reference image) are usually displayed to perform comparative image reading.

[0040] The manner in which the images are displayed on the CRTs is registered in a CRT image display control table as shown in Fig. 14. The table is formed by associating the examination ID and the image ID with the serial number of the CRTs. The table is stored in the semiconductor memory 86.

[0041] The image data which are sequentially transferred to the workstation 14 from the data base 12 are sequentially processed with a predetermined CAD algorithm.

[0042] A timing at which the CAD operation is started will be described below. After image data, examination data, and relevant data of one patient are transferred to the HD unit 106 of the workstation 14, the examination data and relevant data are read out sequentially from the HD unit 106 to the semiconductor memory 86 by the CPU 88.

[0043] Since the CAD operation is performed in which one of a plurality of different CAD algorithms suitable for the image data is selected, the ROM 92 includes a table indicating the name of a CAD algorithm and the items of the attribute data of the image data capable of being applied with the CAD algorithm, as shown in Fig. 15. The items of the attribute data of the image data to be analyzed and corresponding items of the attribute data of each CAD algorithm included in the table shown in Fig. 15 are compared with each other to determine whether or not the CAD algorithm can be applied to the image data. For example, a CAD algorithm for an interstitial lung disease is performed only when the modality

is a conventional radiograph, the examination object is a chest, the imaging direction is a front, and the result of CAD is nothing. If the CAD algorithm is not applied to the image data, nothing is stored in the item of the result of CAD. If other than nothing is stored in the item of the result of CAD, it means that the CAD algorithm is used for the image data. Therefore, since the examination data (Fig. 2) and the relevant data (Fig. 6) are already read out into the semiconductor memory 86, the items of modality and examination object are extracted from the examination data, and the items of imaging direction and result of CAD are extracted from the relevant data. These items are compared with items for each algorithm stored in the table shown in Fig. 15. The table of Fig. 15 is read out from the ROM 92 and is stored in the semiconductor memory 86. If they are equal to each other, the image is determined to be an object to which the CAD algorithm is to be applied. Therefore, an arithmetic operation of the CAD algorithm corresponding to the image data is started.

[0044] First, the image data determined to be an object to which the CAD algorithm is to be applied is read out into the semiconductor memory 86. The CPU 88 executes the CAD algorithm stored in the ROM 92 and stores the result of CAD in the semiconductor memory 86. The CPU 88 issues a serial number for the CAD ID and writes the CAD ID for retrieving the result of CAD in the item of the result of CAD in the relevant data (Fig. 6) stored in the semiconductor memory 86. The CPU 88 also writes the address storing the result of CAD in the relevant data. The default data of the address of the result of CAD is text data denoting nothing. When the operation for one CAD algorithm is ended, it is determined whether the next CAD algorithm can be applied to the image data.

[0045] The examples of the CAD algorithm written in the ROM 92 are as follows. A CAD algorithm for detecting a micro calcification in mammography is disclosed in Unexamined Japanese Patent Application No. 2-152443. A CAD algorithm for measuring the size of the heart and lung is disclosed in United States Patent Application No. 275,720 (filed November 23, 1988). A CAD algorithm for detecting an interstitial lung disease is formed of the following algorithms:

#1: An algorithm (which is schematically shown in Fig. 17, and illustrated in detail in Fig. 18) for setting ROIs (symbolized by □ in Fig. 16) for the CAD algorithm for one frame of the image data.

#2: An algorithm (which is schematically shown in Fig. 19) for calculating a physical amount of texture (which is an index indicating the magnitude and the length of period of a density variation in a texture pattern) in the ROI.

#3: An algorithm (the flow chart of which is shown in Fig. 20, and the arrangement in Fig. 21) for applying a threshold to the calculated physical amount of texture to determine abnormality or normality of

the ROI.

[0046] Of these algorithms, the algorithms #1 and #2 are described in USP 4,851,984, and therefore a detailed description thereof will be omitted. In addition, since the algorithms #3 is described in USP 4,839,807, a detailed description thereof will be omitted.

[0047] The results of the CAD algorithm and the classification of the normality are temporarily stored in the semiconductor memory 86. The detailed description for the case of the interstitial lung disease will be described. It is to be noted that "diffuse" is determined for those classified to be abnormal (i.e., those determined to be clustered abnormal ROIs in the flowchart shown in Fig. 20) because of the presence of clusters (grouped abnormal ROIs), and "local" is determined for abnormalities other than these; they are called patterns of abnormality. The pattern of abnormality is included as one item in the result of CAD of Fig. 22, and the type of pattern is written in this item as text characters, e.g., denoting local. Fig. 23 shows a practical example of the result of CAD in the case of an abnormal ROI. Here, a TPF represents a true positive fraction and an FPF represents a false positive fraction. The ID of the result of CAD and the address of this CAD result data in the semiconductor memory 86 are additionally written as items in the relevant data (Fig. 5). When the result of CAD is stored in the data base 12, the ID and address are registered in the examination directory as shown in Fig. 9. The above operation is performed plural times if plural CAD algorithms can be applied to the image data. If plural results of CAD and addresses are obtained, all the plural IDs and addresses are stored in the examination directory.

[0048] The CAD result is output in response to application of an output request trigger. Therefore, while image reading is performed (a conventional X-ray radiograph of a chest is read or viewed in case of interstitial lung disease detection CAD), various commands including this output request must be input from the input device 80 of the workstation 14. In this embodiment, the description of the input device 80 will be given by using a touch panel type device. It is also possible to use a general device, such as a keyboard as the input device 80.

[0049] Fig. 24 shows an example of the input device 80. This touch panel comprises a command display 110 on which the names of commands is displayed, a panel 112 on which the command display 110 is arranged, and a transparent sensor board 114 located on the command display 110. When a position corresponding to the name of a command is selectively touched with a finger, the sensor board 114 senses the touched portion.

[0050] When, for example, several command buttons are displayed on the output device, an operator can recognize a command display through the sensor board 114. The operator selects a command by touching the sensor board 114, thus executing the command. A but-

ton (CAD button shown in Fig. 25) for requesting an output of a result of CAD is prepared (displayed) on the touch panel. Detecting depression on this CAD button on the touch panel is a trigger for requesting the CAD result output.

[0051] Since the CAD result can be output in various modes, the mode of outputting the CAD result is determined next. The CPU 88 reads out the relevant data (Fig. 6) corresponding to the examination ID and image ID included in the CRT image display control table (Fig. 14). Further, the CPU 88 reads out the CAD result ID and CAD result address from this relevant data, thereby reading out or retrieves the result of CAD (Fig. 22).

[0052] An example of CAD result output is described below. The CPU 88 starts the program in the ROM 92 and outputs a CAD result (Fig. 23) relating to the abnormality to a corresponding output device according to the pattern of the abnormality. In this program, the item of data denoting the pattern of abnormality is extracted from the result of CAD (Fig. 23) relating to the abnormality and stored in the semiconductor memory 86. If the pattern of abnormality is a diffused pattern, a text sentence generator is activated in order to output an abnormality alarm in the form of a text sentence. If the pattern of abnormality indicates local, the alarm (marker) generator 83 is activated in order to indicate the location of abnormality by means of a marker.

[0053] In this case, the text sentence represents the location of abnormality on an image by means of words, thereby making an alarm. For this purpose, as shown in Fig. 26, a screen of the display is equally divided into six regions in advance, and a name is assigned to each region. A table (Fig. 27) showing a correspondence between the names and the x, y coordinates of the regions is stored in the ROM 92. The right and left is defined as viewed from the patient. The CPU 88 starts the program in the ROM 92. In this program, the x, y coordinates of the location of the abnormal ROI is extracted from the CAD result and an expression of abnormality is read out from the table shown in Fig. 28 and stored in the ROM 92 in accordance with the location of the abnormality. The readout expression data is stored in the semiconductor memory 86 to be inserted into the text sentence. If plural CAD results are obtained, the above operation is repeated for the number of the CAD results. The text sentence is, for example, "interstitial lung disease, upper right lung abnormal." In this case, the expression of the underlined portion changes in accordance with an abnormal portion. Subsequently, character string data of the text sentence is converted into dot patterns in units of characters. Thereafter, with reference to the CRT image display control table (Fig. 14), one text line (white) is provided in the uppermost stage of an image memory 100 (overlay screen) corresponding to the CRT displaying the image, and dot patterns of black characters are stored in the text line of the image memory 100, as shown in Fig. 29.

[0054] The marker is a means for representing the lo-

cation of abnormality on an image by using an arrow. The CPU 88 of the workstation 14 starts the program in the ROM 92 and reads out the location of abnormality from the CAD result data (Fig. 22), thus forming the shape of a marker as shown in Fig. 29, based on a font pattern of the ROM 92. In this case, although d (diagonal of the square) = 1.5 cm is preferable, d is not limited to this value but can be changed freely. The screen is divided into right and left portions as viewed from the operator. If the location (the center of ROI indicated by a symbol \times) of abnormality is present on the right side of the screen, the arrow shown in Fig. 30 is converted directly into a bit pattern. If, by contrast, the location is present on the left side, the arrow of Fig. 30 is inverted symmetrically about a longitudinal line (alternate long and short dashed line in Fig. 30) including the center of ROI, i.e., in a mirrorlike manner and the resulting mirror image of the arrow as indicated by a broken line in Fig. 30 is converted into a bit pattern.

[0055] In addition, the bit pattern data is written in a location corresponding to the position of abnormality in the image memory 100 (overlay memory) corresponding to the CRT displaying the image. If a plural CAD results are obtained, the above operation is repeated until all the CAD results are read out and written into the overlay memory. The data in the image memory 100 (overlay memory) is displayed on the CRT overlapped with the image data. The display color of the bit pattern data of the marker is switched between black and white in synchronism with the timer 90. Thus, the effect of alarming of the marker is enhanced. It is noted that the period of switching is 2Hz.

[0056] At this time, though all the CAD results are simultaneously displayed on the CRT, some of them may be selectively displayed. The names of buttons displayed on the touch panel are changed in accordance with the needs of the operator. For example, the names of the buttons are changed in accordance with the CAD algorithm now applying to the image data. A label "ID", "MC", and "BH" are provided for buttons in case of an interstitial lung disease detection CAD, micro calcification detection CAD, and heart size measuring CAD. When a CAD algorithm is selected, the CAD result corresponding to the algorithm is written in the overlay memory and the other results are deleted from the overlay memory.

[0057] Another mode of CAD result output will be described in which the CAD result has a hierarchical structure. That is, a summary of the CAD result is output first by means of, e.g., the text sentence and the marker as described above, and then details are output. For this purpose, a button for requesting a CAD detail output is prepared on the input device (touch panel) 80 (Fig. 25) of the workstation 14. In other words, the names of buttons on the touch panel are changed in accordance with the application used by an operator. When depression on the CAD detail output button on the touch panel is sensed while the text sentence and the marker are dis-

played, a trigger for requesting an output of the CAD detailed result is generated.

[0058] The output of the CAD detailed result will be described below. It is assumed that the text sentence is already formed and stored in the form of black characters on a white background as shown in Fig. 29 in the image memory 100 (overlay screen). The CPU 88 starts the program in the ROM 92 to read out the CAD result data (Fig. 22) from the semiconductor memory 86. The CPU 88 forms an arrow marker for data having abnormality independently of the pattern of the abnormality. The marker indicates the location of the abnormality on an image by means of an arrow.

[0059] The CPU 88 reads out the location of the abnormality and forms the shape of the marker as shown in Fig. 31, based on the font pattern in the ROM 92. At this time, the screen is divided into right and left portions. If the abnormality location is present on the right side viewed from the operator, the arrow of Fig. 31 is converted directly into a bit pattern. If, on the other hand, the abnormality location is present on the left side, the arrow of Fig. 31 is mirrorlike-inverted symmetrically about a longitudinal line (alternate long and short dashed line in Fig. 31) including the location of the abnormality, and the resultant mirrorlike arrow as indicated by a broken line in Fig. 31 is converted into a bit pattern. In addition, the type (e.g., nodular) and the degree (e.g., 75%) of the abnormality are read out from the CAD result data and are converted into a bit pattern, as shown in Fig. 31. Unlike the bit pattern of the arrow, the bit pattern of characters of the type and degree is not mirrorlike-inverted regardless of whether the abnormality location is present on the right side or the left side.

[0060] This bit pattern data is written in a location corresponding to the position of the abnormality in the image memory 100 (overlay screen) corresponding to the CRT 102 displaying the image. As a result, the arrow marker associated with the characters indicating the type and the degree of the abnormality (Fig. 31) is displayed, together with the text sentence shown in Fig. 29, on the screen.

[0061] The data in the image memory 100 (overlay screen) is displayed overlapped on the examination image. At this time, the color of the data display on the overlay screen is switched between black and white in synchronism with the timer 90. The period of switching is 2Hz.

[0062] An example of an option output of the CAD detailed result will be described below. As in the case of the trigger for the detailed output, a button for requesting a detailed option output of the CAD result is displayed on the input device (touch panel) 80 of the workstation 14 as a trigger for the option output. When depression on the CAD detailed option output button on the touch panel is sensed while the detailed output is performed, the trigger for requesting the CAD detailed option output is attained.

[0063] It is supposed that the text sentence is already

formed and stored in the form of black characters on a white background as shown in Fig. 29 in the image memory 100 (overlay screen). The CPU 88 starts the program in the ROM 92 to read out the CAD result data (Fig. 22) from the semiconductor memory 86 and forms an arrow marker for data having abnormality independently of the pattern of the abnormality. This marker represents the location of the abnormality on the image by means of an arrow.

[0064] The CPU 88 reads out the location of the abnormality and forms an arrow marker and a square ROI marker, as shown in Fig. 32, based on the font pattern of the ROM 92. Here, the screen is divided into right and left portions. If the abnormality location is present on the right side, the arrow and the ROI of Fig. 32 are converted directly into bit patterns. If the location is present on the left side, the arrow of Fig. 32 is inverted in a mirrorlike manner, and the resulting arrow indicated by a broken line in Fig. 32 and the ROI are converted into bit patterns. This bit pattern data is written in the location corresponding to the position of the abnormality in the image memory 100 (overlay screen) corresponding to the CRT displaying the image in the CRT display image control table (Fig. 12).

[0065] The data in the image memory 100 (overlay screen) is displayed overlapped on the examination image. At this time, the color of the data display on the overlay screen is switched between black and white in synchronism with the timer 90. The period of switching is 2Hz.

[0066] Another example of the option output will be described. When another option output is requested, the CPU 88 starts a given program in the ROM 92 to read out ROC (Receiver Operator Curve) data included in the CAD result from the semiconductor memory 86, thus forming an ROC curve. As shown in Fig. 33, the ROC curve is one of examples for indicating the ability of CAD and is so formed as to be fitted in a portion below and to the right of the image. In the ROC curve, the abscissa denotes the FPF and the ordinate denotes the TPF. The ROC curve is converted into a bit pattern. The bit pattern data is written in the image memory 100 (overlay screen) corresponding to the CRT displaying the image. The data in the image memory (overlay memory) 100 is displayed on the CRT overlapped with the examination image.

[0067] An example of a request trigger for ending the output of the CAD result will be described below. When the image reading of a conventional X-ray radiograph of a chest is performed and the image and the CAD result are displayed on a CRT screen, the trigger for ending the CAD result output is automatically generated upon stopping the image display in order to display another image. When the output is ended, the image display is continued, and only the display on the overlay screen is turned off. Further, the touch panel may include a button for providing the command representing the end of the image reading and the relevant data is updated as being

read if the button is depressed.

[0068] A command for requesting the end of the CAD output can also be applied from the input device 80 of touch panel type.

[0069] It is to be noted that the CAD data is preferably stored even when its output (display) is stopped. The CAD result is added to the updated relevant data, as shown in Fig. 34, and supplied to the data base 12 to be stored therein. In the data base 12, all the CAD IDs and CAD result addresses in the relevant data are stored in the examination directory (Fig. 9). In a subsequent image reading, if an image transfer request is supplied to the data base 12, the image data and the corresponding examination and relevant data are transferred by the network 16 and stored in the semiconductor memory 86 of the workstation 14. At the same time, the CAD result ID is read out and all the CAD results are retrieved based on the CAD IDs. In this case, as shown in Fig. 35, the address of the CAD result written in the relevant data is converted into the address on the semiconductor memory 86 and is stored in the relevant data.

[0070] According to this embodiment as has been described above, the following effects can be obtained. That is, in addition to a medical image, CAD data concerning the image is also displayed. Therefore, an erroneous diagnosis due to an oversight of a disease can be prevented in medical image diagnosis, thus increasing diagnosis precision. Labors can be reduced in a diagnosis operation performed by a doctor (operator). In medical image diagnosis, particularly in an image reading operation, an erroneous diagnosis caused by an oversight of a disease can be prevented to improve diagnosis precision. Since the CAD data is obtained by analyzing medical images using a computer, objective and quantitative results can be obtained. Therefore, it is possible to prevent an erroneous diagnosis which is a result of subjective determination by a human being, and consequently diagnosis precision can be increased. In medical image diagnosis, a doctor who is not an expert of an image of interest sometimes cannot make a satisfactory diagnosis. According to the present invention, diagnosis precision can be improved also in this case.

[0071] As the CAD data, the position, the type, or the degree of abnormality is displayed, so that the abnormality can be readily recognized. As a result, an erroneous diagnosis caused by an oversight of a disease can be prevented to improve diagnosis precision.

[0072] Arithmetic operation calculating the CAD data is started by a computer before an output request for the CAD data is generated. Therefore, it is possible to shorten a time from generating the output request to displaying the CAD data.

[0073] When several algorithms for obtaining CAD data are available, an inappropriate processing is performed for an image data of interest unless the image data is correctly assigned to the algorithm, and erroneous CAD data results. According to this embodiment,

however, since a suitable algorithm is selected for each image, output of erroneous CAD data can be prevented to increase diagnosis precision.

[0074] Since the CAD result is stored in the data base 12, an image which is diagnosed once need not be analyzed again.

[0075] A CAD algorithm is determined for each diagnosis of interest, and the algorithms are selectively executed in accordance with each object. Therefore, it is possible to prevent a production of CAD data which may cause an erroneous diagnosis in the case when an unsuitable algorithm is applied to an object. Further, the attribute data includes the modality, the examining object, and the imaging direction, and an algorithm is executed when these items of the attribute data coincide with those of an object image of the algorithm. Therefore, an unsuitable algorithm is not applied to the image.

[0076] An alarming means which strongly attracts attention of the doctor is used as a means for alarming abnormality. Therefore, an erroneous diagnosis due to an oversight can be prevented to increase diagnosis precision. An optimal alarming means is selected to attract attention in accordance with the type of abnormality. Therefore, it is possible to prevent an erroneous diagnosis caused by an oversight, thus improving diagnosis precision. By flickering the alarm display, the alarming means strongly attracts attention to prevent an erroneous diagnosis resulting from an oversight, thus improving diagnosis precision.

[0077] The CAD data is hierarchically constructed and output gradually from its summary to details. Therefore, a large number of different types of CAD data are not simultaneously displayed to cause a cumbersome operation. Thus, an erroneous diagnosis can be prevented to increase diagnosis precision. For example, the position of abnormality alone is output first as the CAD data. If the abnormality cannot be clearly determined, a doctor freely makes output requests for, e.g., the degree, the type, and the pattern of the abnormality, thus avoiding a cumbersome operation to increase diagnosis precision. In this case, a usable command (button) is prepared for each level (hierarchical level) of contents at which the CAD data is output. Since a user need only select a command of interest from the prepared commands, a labor for selecting from a large number of commands is reduced.

[0078] Before application of the CAD algorithm to a given image data, it is determined whether the CAD algorithm can be applied to the image data based on the attribute data of the image data and only the algorithm which is determined to be able to apply to the image data is applied to the image data. Therefore, it is possible to prevent lowering the quality and precision of diagnosis due to the output of the erroneous CAD data.

[0079] The CAD system according to the present invention is described as being incorporated into the PACS. However, it is possible to realize a stand-alone type CAD system according to the present invention.

[0080] Plural CAD algorithms are stored in the system and an optimum one is automatically selected based on the relevant data of the object image data. Therefore, it is possible to reduce the labors of the doctor for selecting the suitable algorithm, inputting the respective image data, and outputting the respective CAD data.

[0081] The computer starts an arithmetic operation for calculating the CAD data before an output request for the CAD data is generated. Therefore, it is possible to shorten a time from generating the output request to displaying the CAD data.

[0082] The numerical data denoting the CAD result includes many items. If all the data are output, the output becomes complicate. According to the first embodiment, the CAD data are stored in the form of a table and only desired data is output by retrieving the data from the table using the retrieval key corresponding to the desired condition. Therefore, the CAD result can be output in a simple form.

[0083] The attribute data includes an item of data denoting whether or not the image data has been read or viewed. Based on this attribute data, the CAD result of the image data which has been read or viewed is not output. Therefore, it is possible to prevent a confusion in which the CAD result different from the reading report is output. Based on this attribute data, only the image data which has not been read or viewed is analyzed using the CAD algorithm. Therefore, a time from generating the output request to displaying the CAD data becomes shorter than that in the case of all the image data are analyzed. Further, the attribute data includes an item of data representing the CAD result and the image data which has been analyzed is not analyzed again. Therefore, it is possible to further shorten a time from generating the output request to displaying the CAD data.

[0084] Other embodiments of the present invention will be described below.

[0085] A second embodiment comprises, in addition to the workstation 14 for displaying the image as shown in Fig. 12, a workstation 14a having a CAD processor 120 as shown in Fig. 36. This workstation 14a for obtaining CAD data is different from the workstation 14 in that a controller 90a is provided in place of the timer 90. In terms of an operation, the second embodiment is different from the first embodiment in a timing at which a CAD arithmetic operation is started.

[0086] In the second embodiment, when image data, examination data, and relevant data of one patient are transferred to the HD unit 106 of the workstation 14a, the examination data and the relevant data are read out sequentially from the HD unit 106 into the semiconductor memory 86 by the CPU 88. The ROM 92 stores the table denoting the relationship between the name of the CAD algorithm and the attribute data of the image data which can be adapted to the CAD algorithm as shown in Fig. 15. Therefore, since the examination data (Fig. 2) and the relevant data (Fig. 6) are already read out into the semiconductor memory 86, the modality and the

examining object are read out from the examination data, and the imaging direction is read out from the relevant data. These read out items of data are stored in the semiconductor memory 86. These items of data are compared with the attribute data of the image stored in the table (Fig. 15) of the ROM 92.

[0087] If these items are coincide with those of a given CAD algorithm, e.g., interstitial lung disease detection CAD, this image is determined to be an image to which the interstitial lung disease detection CAD algorithm can be applied, and the operation of the CAD is started. At this time, the CPU 88 in the workstation 14a designates activation of the CAD processor 120 (Fig. 36), and supplies input data to the processor 120. The input data given to the CAD processor 120 includes the image data, the examination data, and the relevant data. The CAD processor 120 has its own CPU, and by means of the CPU it executes the CAD operation and outputs a CAD result. The CAD result is temporarily stored in the memory as data having the format shown in Fig. 22. In addition, the ID and the address of the CAD result data are additionally written in the relevant data (Fig. 6).

[0088] As described above, according to the second embodiment, since the display and the CAD arithmetic operation are separately performed at different workstations 14 and 14a, a processing time for the CAD can be shortened. That is, if a CAD processing is performed at devices such as the modality 10, the workstation 14, and the data base 12, a long processing time is required for they share a single CPU. However, since the CAD processor 120 has a CPU 88 for a processing purpose only, the processing time is shortened.

[0089] A third embodiment is different from the first embodiment in that a CAD result is output as a sound. For this purpose, a workstation of this embodiment has a sound generator as shown in Fig. 37 in addition to the arrangement shown in Fig. 10. The CPU 88 of the workstation 14 reads out relevant data using the CRT image display control table (Fig. 14). The CPU 88 also reads out CAD results (Fig. 22) by reading out the CAD result address from the relevant data. When the CAD result is to be output, the CPU 88 starts a program in the ROM 92 and assigns the CAD result having abnormality to a corresponding output device in accordance with the pattern of the abnormality. In this program, the CAD results and the classification of the CAD result are read out from the semiconductor memory 86, and, if the type of abnormality indicates "diffuse", a text sentence generator is activated in order to output an abnormality alarm in the form of a text sentence. If the type of abnormality indicates "local", a marker generator and the sound generator shown in Fig. 37 are activated in order to indicate the position of the abnormality by means of a marker and a sound.

[0090] When the CAD operation result is read out from the semiconductor memory 86, if the pattern of abnormality indicates "local", a sound of "abnormality present" is simply generated. If, however, the pattern of

abnormality indicates "diffuse", a statement formed as a text sentence is automatically read. The text sentence is, for example, "interstitial lung disease, upper right lung abnormal." The expression in the underlined portion changes in accordance with an abnormal portion. Next, the CPU 88 activates a program in the ROM 122 and converts character string data in the text sentence into a voice sound. "Interstitial lung disease, upper right lung abnormal" is stated by generating three groups of words, interstitial lung disease, upper right lung, and abnormal. Since the expression in the underlined portion changes in accordance with an abnormal portion as described above, a sound data base 124 is also provided to generate words for this purpose.

[0091] According to the third embodiment as described above, in specifying the position of abnormality by means of a sentence or a sound, words representing a position are used to make it easy to recognize the abnormality. Therefore, an oversight of a disease and consequently an erroneous diagnosis can be prevented to lead to an increase in diagnosis precision.

[0092] As a fourth embodiment, an embodiment of automatically outputting a CAD result will be explained. The arrangement of a workstation of the fourth embodiment is identical to that of the first embodiment shown in Fig. 12. In the fourth embodiment, however, even if no CAD result request is present during image reading of a conventional X-ray radiograph of chest, the result is automatically displayed.

[0093] For this purpose, each time an image is displayed, the CPU 88 refers to the CRT image display control table (Fig. 14) and checks whether the ID of the CAD result is included in the relevant data of the displayed image, i.e., whether nothing is stored in the CAD result ID, and in this manner checks whether the displayed image is an object of the CAD. If the CPU 88 determines that the displayed image is an object of the CAD, it measures a predetermined time from the start of image display by means of the timer 90, and automatically generates a trigger for requesting a CAD result output when the predetermined time has elapsed. This predetermined time can be arbitrarily changed.

[0094] In this manner, the output request for the CAD data can be omitted, and this results in a reduction in labors. In addition, if the CAD data is output immediately after an image is displayed, an operator or doctor may have a preconceived knowledge. Therefore, CAD data is output when a certain time has elapsed after an image is displayed. As a consequence, an erroneous diagnosis due to an oversight is prevented to improve diagnosis precision.

[0095] A fifth embodiment as another example of automatically outputting the CAD result will be described. Here, the arrangement of a workstation of this embodiment is also the same as that shown in Fig. 12. First, each time an image is displayed, the CPU 88 refers to the CRT image display control table (Fig. 14) and checks whether the ID of the CAD result is included in

the relevant data of the displayed image, i.e., whether nothing is stored in the CAD result ID, and in this manner checks whether the displayed image is an object of the CAD. If the CPU 88 determines that the displayed image is an object of the CAD, it measures a number of times (the number of applications of the CAD algorithm) at which the image is displayed from the start of the image reading for the patient and writes the number of times into the relevant data (Fig. 6). The number of times is initially set to zero and increased by one every time the image is displayed. The CPU 88 automatically generates a trigger for requesting a CAD result output when the number of times reaches a predetermined time which can be arbitrarily set.

[0096] In this manner, since an output request for CAD data can be omitted, labors can be reduced. In addition, if CAD data is output immediately after an image is displayed, an operator or doctor may have a preoccupied knowledge. Therefore, CAD data is not output when an image is displayed for the first time and image reading is performed but output when the image is displayed for a predetermined time or the image display is switched. The result is that an erroneous diagnosis caused by an oversight is prevented to improve diagnosis precision.

[0097] The fourth and fifth embodiments are embodiments automatically outputting a CAD result. Next, a sixth embodiment of automatically ending outputting of a CAD result will be described. The arrangement of a workstation of this embodiment is identical to that shown in Fig. 12. When, for example, image reading of a conventional radiograph of a chest is performed, a display of the CAD result is automatically stopped even if no CAD result request is present. For this purpose, each time an image is displayed, the CPU 88 refers to the CRT image display control table (Fig. 14) and checks whether the ID of the CAD result is included in the relevant data of the displayed image, i.e., whether nothing is stored in the CAD result ID, and in this manner checks whether the displayed image is an object of the CAD. If the CPU 88 determines that the displayed image is an object of the CAD, it measures a predetermined time from the start of image display by means of the timer 90, and automatically generates a trigger for requesting the end of the CAD result output when the predetermined time has elapsed. This predetermined time can be arbitrarily changed. Upon the end of outputting, the CPU 88 turns off all overlay screens displayed on CRTs.

[0098] According to this embodiment, since an output end request for CAD data can be omitted, labors are reduced. In addition, CAD data remaining on an image for a long time makes it difficult for an operator or doctor to observe details of an image. As in this embodiment, however, by automatically ending display of CAD data after the data has been displayed for a predetermined time, an erroneous diagnosis is prevented to increase diagnosis precision.

[0099] Various commands must be input in the

present invention, so a seventh embodiment relating to a modification of the input device will be described below. During image reading of a conventional radiograph of a chest, when an icon displayed on a CRT screen is designated (clicked) by a pointing device such as a mouse, a menu window as shown in Fig. 38A appears at a corner, in this case, the upper right corner of the screen. It is to be noted that this menu window shows only buttons which can be used by an operator at the time of click. If it is electrically sensed that a CAD button in the menu window on the screen is designated by the pointing device, a trigger for requesting a CAD result output is generated.

[0100] Similarly, when the icon displayed on the CRT screen is designated (clicked) by the pointing device such as a mouse, as shown in Fig. 38B, while the CAD output is performed, the menu window emerges. If a button for requesting a CAD detail result output in the menu window is designated, a trigger for requesting the CAD detail result output is generated. When the icon displayed on the CRT screen is designated (clicked) by the pointing device such as a mouse while the CAD output is performed, the menu window appears. If a button for requesting an option output in the menu window is designated, a trigger for requesting an option output is generated. When the icon displayed on the CRT screen is designated (clicked) by the pointing device such as a mouse while the CAD output is performed, the menu window emerges. If a button for requesting a CAD diagnosis level output in the menu window is designated, a trigger for requesting the CAD diagnosis level output is generated. When the icon displayed on the CRT screen is designated (clicked) by the pointing device such as a mouse while the CAD output is performed, the menu window appears. If a button for requesting a CAD result output end in the menu window is designated, a trigger for requesting the CAD detail output end is generated. Upon the end of outputting, overlay screens are turned off.

[0101] According to this embodiment as described above, a menu window including buttons having command names is displayed on the CRT screen. By designating a command with by means of a pointing device such as a mouse, a command for outputting CAD data can be input. In addition, since the menu window is not constantly displayed but can be selectively displayed, an operator (doctor) can display commands only when he or she needs them. Therefore, an annoyance caused by frequent changes in commands displayed can be reduced. In this case, a usable menu is prepared for each level (hierarchical level) of the contents of CAD data to be output. Therefore, since a user need only select a menu of interest from the prepared menus, a labor of selecting from a large number of menus is reduced.

[0102] An eighth embodiment concerned with coloring of a marker and a text sentence will be described below. The arrangement of a workstation is the same as that shown in Fig. 12. With reference to the CRT image

display control table (Fig. 14), an overlay screen corresponding to a CRT not having "nothing" in the ID of the CAD result of relevant data of a displayed image is overlaid on the examination image displayed on the CRT. At this time, the data displayed on the overlay screen is flickered in an arbitrary color, such as red, while being synchronized by the timer 90. The period of flickering is 2 Hz.

[0103] According to the eighth embodiment, it is possible to strongly attract attention because of the color of the alarm display. As a result, an erroneous diagnosis caused by an oversight can be prevented to consequently increase diagnosis precision. This effect can be further enhanced by flickering the alarm display.

[0104] A ninth embodiment in which a CAD arithmetic operation is started by the modality, such as a film digitizer 18 (Fig. 4) will be described. The arrangement of a workstation is identical to that shown in Fig. 12. In this embodiment, when the film digitizer 18 digitizes all the image data for one patient and inputs the imaging direction, the CPU 88 reads out examination data and relevant data sequentially from the HD unit 106 into the semiconductor memory 86. In order to refer to the table (Fig. 15) of CAD algorithms and corresponding attribute data, the modality and the examination object are read out from the examination data (Fig. 2) and the imaging direction and the CAD result ID address are read out from the relevant data (Fig. 6). These readout items of data are stored in the semiconductor memory 86. These items of data are compared with the attribute data of the image stored in the table (Fig. 15) of the ROM 92. If these items are coincide with those of a given CAD algorithm, this image is determined to be an image to which the given CAD algorithm can be applied, and the operation of the CAD is started.

[0105] Upon the start of the CAD operation, image data determined to be an object of the CAD is read out into the semiconductor memory 86. The CPU 88 executes a CAD operation program written in the ROM 92 and stores the result in the semiconductor memory 86. The CPU 88 transfers, as data flowing through the network 16, the image data, the relevant data, the CAD result, and the examination data (for each examination) to the data base 12 via the LAN I/F 94. As shown in Fig. 34, the data base 12 handles the CAD result data as a part of the relevant data.

[0106] When data is transferred to the workstation 14 during image reading, the transferred data is temporarily stored in the HD unit 106. However, the CAD result is read out from the HD unit 106 into the semiconductor memory 86 upon reception of a CAD output request as a trigger. In this case, the workstation 14 does not perform any operation associated with the CAD but simply displays the CAD result. Whenever an image is displayed on the image display device (workstation), the CAD result for the displayed image is stored in the semiconductor memory 86. Therefore, a time from generation of an output request to display the CAD result is

shortened.

[0107] In a tenth embodiment, a timing at which an arithmetic operation of a CAD is started is when all the image data of one patient is transferred to the data base 12. At this time, the CPU 88 reads out examination data and relevant data sequentially from the HD unit 106 into the semiconductor memory 86. In order to refer to the table (Fig. 15) of CAD algorithms and corresponding attribute data, the modality and the examination object are read out from the examination data (Fig. 2) and the imaging direction and the CAD result ID address are read out from the relevant data (Fig. 6). These readout items of data are stored in the semiconductor memory 86. These items of data are compared with the attribute data of the image stored in the table (Fig. 15) of the ROM 92. If these items are coincide with those of a given CAD algorithm, this image is determined to be an image to which the given CAD algorithm can be applied, and the operation of the CAD is started.

[0108] Upon the start of the CAD operation, image data determined to be an object of the CAD is read out into the semiconductor memory 86. The CPU 88 executes a CAD operation program written in the ROM 92 and stores the result in the semiconductor memory 86. The CPU 88 transfers, as data flowing through the network 16, the image data, the relevant data, the CAD result, and the examination data (for each examination) to the data base 12 via the LAN I/F 94. As shown in Fig. 34, the data base 12 handles the CAD result data as a part of the relevant data.

[0109] When data is transferred to the workstation 14 during image reading, the transferred data is temporarily stored in the HD unit 106. However, the CAD result is read out from the HD unit 106 into the semiconductor memory 86 upon reception of a CAD output request as a trigger. In this case, the workstation 14 does not perform any operation associated with the CAD but simply displays the CAD result. Whenever an image is displayed on the image display device (workstation), the CAD result for the displayed image is stored in the semiconductor memory 86. Therefore, a time from generation of an output request to display the CAD result is shortened.

[0110] Fig. 39 is a block diagram showing the arrangement of an eleventh embodiment. In the eleventh embodiment, a CAD processor 14a as shown in Fig. 36 is connected to the arrangement of the PACS shown in Fig. 1. When a request of starting a CAD operation is generated in the workstation 14, the CAD processor 14a is used to perform only the CAD operation at a high speed. Therefore, the workstation 14 transfers data required for the CAD operation to the CAD processor 14a, and only the result is returned to the workstation 14.

[0111] A timing at which the CAD operation is started is similar to that in the tenth embodiment. However, unlike in the tenth embodiment, the CAD operation is performed by the CAD processor 14a. The workstation 14 supplies the image data, the examination data, and the

relevant data to the CAD processor 14a via the network 16. As shown in Fig. 36, the CAD processor 14a has its own CPU, and by means of the CPU it executes the CAD operation and outputs the CAD result. The result of the CAD operation is transferred as result data having the format shown in Fig. 22 to the workstation 14 via the network 16. As shown in Fig. 34, the workstation 14 or the data base 12 handles the CAD result as a part of the relevant data.

[0112] When data is transferred to the workstation 14 during image reading, the transferred data is temporarily stored in the HD unit 106. The CAD result, however, is read out from the HD unit 106 into the semiconductor memory 86 upon reception of an output request for the CAD as a trigger. In this case, the workstation 14 does not perform any operation associated with the CAD but simply displays the result.

[0113] Processing executed by devices such as the modality, the workstation, and the data base takes a long processing time for they share a CPU. In this embodiment, however, since the processor having a CPU for a processing purpose only executes the processing, a processing time can be shortened.

[0114] As a twelfth embodiment, an embodiment concerned with a modification of a marker will be described below. Figs. 40A to 40E show modifications of a marker for pointing the ROI, and Figs. 41A to 41F show modifications of a marker for surrounding the ROI. Pointing the ROI includes a case in which the direction of an arrow points the center of the ROI as shown in Fig. 42A and a case in which it points a position other than the center as shown in Fig. 42B.

[0115] According to this embodiment, an alarming means which strongly attracts attention is used in order to alarm abnormality. Therefore, an oversight and therefore an erroneous diagnosis can be prevented, and this results in an improvement in diagnosis precision.

[0116] A thirteenth embodiment in which an on/off of the CAD result display is controlled for each of the CRTs will be described. The touch panel includes plural CAD result display buttons provided for the respective CRTs. In order to display only the CAD result on the CRT #1, it is necessary to depress the CAD result display buttons for the CRT #1. When the depression of that button is detected, the ID of the image displayed on the CRT #1 is read out from the CRT display control table (Fig. 14). The CAD result address is read out from the relevant data of the image and the CAD result data is written into the overlay memory for the CRT #1, thereby displaying the CAD result overlapped on the image. As described above, the operation of this embodiment is the same as that of the first embodiment except that the image ID is read out from the CRT display control table. If no CAD result address is stored (nothing is stored in the CAD result ID), the same operation as the first embodiment is performed from application of a suitable CAD algorithm to the image data to writing the CAD result address into the table.

[0117] According to the thirteenth embodiment, only necessary CAD results are selectively displayed during the reading of the images displayed on the CRTs of the workstation, therefore, the display is not complicate due to the omission of display of unnecessary CAD result.

[0118] A fourteenth embodiment which is a modification of the thirteenth embodiment will be described. In this embodiment, when the image ID of the CRT display control table is updated upon changing the image to be displayed, the CAD result address is read out from the relevant data of the new image and the CAD result is written into the overlay memory, thereby displaying the CAD result overlapped on the image. That is, when the image ID is designated, the CAD result is automatically displayed regardless of whether or not the image has been read. If no CAD result address is stored (nothing is stored in the CAD result ID), the same operation as the first embodiment is performed from application of a suitable CAD algorithm to the image data to writing the CAD result address into the table. When the depression of the CAD display button for a reference image (an image other than the image which has been read), the IDs of the images displayed on the CRTs are read out from the CRT display control table (Fig. 14) and it is determined whether or not the image has been read. If the image has been read, the CAD result address is read out from the relevant data and the CAD result is written into the overlay memory, thereby displaying the CAD result overlapped on the image. For all the CRTs, this operation is performed. It is to be noted that all the data in the overlay memory are deleted before the CAD result is written into the memory.

[0119] According to the fourteenth embodiment, since the CAD result is automatically output upon changing the image to be displayed, labors for instructing the CAD result output. It is possible to make a comparison diagnosis with reference to the reference image which has been read, thereby improving the diagnosis precision.

[0120] A fifteenth embodiment as a modification of the thirteenth embodiment will be described. The touch panel includes a single CAD result display button provided for all the CRTs. When the depression of the display button is detected, the IDs of the images displayed on the CRTs are read out from the CRT display control table (Fig. 14). The CAD result addresses for all the images are read out from the relevant data and the CAD result data are written into the overlay memories for all the CRTs, thereby displaying the CAD results overlapped on the images. The CAD results are automatically displayed regardless of whether or not the images have been read. If no CAD result address is stored (nothing is stored in the CAD result ID), the same operation as the first embodiment is performed from application of a suitable CAD algorithm to the image data to writing the CAD result address into the table.

[0121] According to the fifteenth embodiment, since it is possible to make a comparison diagnosis with reference to the reference image which has been read, there-

by improving the diagnosis precision. When the CAD result display is desired, it is sufficient to touch only one button so that the operation is simple.

[0122] A sixteenth embodiment which is a further modification of the thirteenth embodiment will be described. The touch panel includes a CAD result display button for the image which has not been read and a CAD result display button for the reference image (an image other than the image which has not been read). When the depression of the CAD result display button for the image which has not been read is detected, the IDs of the images displayed on the CRTs are read out from the CRT display control table (Fig. 14). It is determined whether or not the image has not been read based on the relevant data of the image. If the image is detected as being not read, the CAD result address is read out from the relevant data of the image and the CAD result data is written into the overlay memory. All the data in the overlay memory are deleted before the CAD result is written into the memory. When the depression of the CAD result display button for the reference image is detected, the IDs of the images displayed on the CRTs are read out from the CRT display control table (Fig. 14). It is determined whether or not the image has not been read based on the relevant data of the image. If the image is detected as being not read, the CAD result address is read out from the relevant data of the image and the CAD result data is written into the overlay memory. All the data in the overlay memory are deleted before the CAD result is written into the memory. If no CAD result address is stored (nothing is stored in the CAD result ID), the same operation as the first embodiment is performed from application of a suitable CAD algorithm to the image data to writing the CAD result address into the table.

[0123] According to the sixteenth embodiment, since it is possible to make a comparison diagnosis with reference to the reference image which has been read, thereby improving the diagnosis precision. When the CAD result display is desired, it is sufficient to touch only one button so that the operation is simple.

[0124] A seventeenth embodiment will be described. Though the above description, a suitable CAD algorithm is selected by the computer using the attribute data, in this embodiment, the doctor designates the name of the CAD algorithm. Before reading of the image, the doctor selects one or more CAD algorithms as well as inputting the examination ID. The names of the selected algorithms are arranged in the form of the table as shown in Fig. 43. When the image is input to the workstation, the CAD algorithms in the table are sequentially applied to the images. The other operation is the same as the first embodiment.

[0125] According to the seventeenth embodiment, only a desired CAD result is selectively displayed and the display becomes simple.

[0126] As has been described above, according to the present invention, there is provided a computer-aided

diagnosis system for medical use, which outputs computer-aided diagnosis data with a high precision by a simple operation having no adverse effect on diagnosis made by doctors and a picture archiving communication system incorporating the computer-aided diagnosis system for medical use and having a high diagnosis precision.

10 Claims

1. A system for analyzing a medical image (14) using a computer-aided diagnosis algorithm, comprising:

interface means (84, 94) for loading a medical image as digital data;

means (86) for storing said medical image data wherein said medical image data comprise attribute image data comprising information related to the type of medical image which can be analyzed by computer aided diagnosis algorithms;

algorithm storing means (92) for storing a plurality of said computer-aided diagnosis algorithms for detecting different types of abnormal portions in the medical image;

means (88) for analyzing the medical image data using one of said plurality of computer-aided diagnosis algorithms to detect abnormal portions in said medical image; and

means for displaying an analysis result of said analyzing means, characterized in that said interface means (84, 94) further comprise means to input said attribute image data of the medical image as digital data;

said analyzing means comprises:

means (92) for storing for each of said plurality of computer aided diagnosis algorithms attribute data defining the type of medical image which can be analyzed by the computer-aided diagnosis algorithm;

means (88) for selecting, based on said attribute data stored in said storing means and said attribute image data of the medical image to be analyzed, an optimum computer aided diagnosis algorithm suitable to analyse said medical image and

wherein said analyzing means analyzes said medical image data using said optimum computer-aided diagnosis algorithm selected by said selecting means.

2. A system according to claim 1, characterized by further comprising:

a network (16) connected to said interface means

data base means (12) connected to said net-

work for storing the medical image data, an analysis result data of said analyzing means, and association data indicating the relationship between the medical image data and the analyzing result data; and
means for writing said analysis result data and said association data into said data base means via said network by means of said interface means.

3. A system according to claim 1 or 2, characterized in that a plurality of modalities are connected to said network.

4. A system according to claim 2, characterized by further comprising:

means (80) for inputting retrieval data to retrieve desired analysis result data stored in said data base means (12); and
means for reading out the analysis result data from said data base means (12) in accordance with said retrieval data.

5. A system according to claim 1 or 2 wherein said attribute image data further comprise information denoting whether or not a medical image has been viewed by a doctor, characterized by further comprising:

means for selectively extracting one of a first plurality of medical images which have been viewed by a doctor and one of second plurality of medical images which have not been viewed by a doctor based on said attribute image data, and characterized in that said analyzing means analyzes said medical images extracted by said extracting means using said optimum selected computer-aided diagnosis algorithm.

6. A system according to claim 2, characterized in that said attribute image data further comprise information denoting whether or not the medical image has been analyzed by said analyzing means.

7. A system according to claim 6, characterized in that said analyzing means analyzes a medical image which has been viewed by a doctor but has not been analyzed by said analyzing means.

8. A system according to anyone of claims 5 to 7, characterized by further comprising display means (82, 100, 102) for displaying the medical image which has not been viewed by a doctor without the analysis result of said analyzing means and displaying the medical image which has been viewed by a doctor with the analysis result.

Patentansprüche

1. System zum Analysieren eines medizinischen Bilds (14) unter Verwendung eines computerunterstützten Diagnosealgorithmus, mit

einer Schnittstelleneinrichtung (84, 94) zum Laden eines medizinischen Bilds in Form von digitalen Daten;

einer Einrichtung (86) zum Speichern der medizinischen Bilddaten, wobei die medizinischen Bilddaten Attributbilddaten enthalten, die mit dem Typ des medizinischen, mittels der computerunterstützten Diagnosealgorithmen analysierbaren Bilds zusammenhängende Informationen aufweisen;

einer Algorithmuspeichereinrichtung (92) zum Speichern einer Mehrzahl der computerunterstützten Diagnosealgorithmen zum Erfassen von unterschiedlichen Arten von abnormalen Abschnitten in dem medizinischen Bild;

einer Einrichtung (88) zum Analysieren der medizinischen Bilddaten unter Verwendung eines aus der Mehrzahl von computerunterstützten Diagnosealgorithmen, um hierdurch einen abnormalen Abschnitt in dem medizinischen Bild zu erfassen; und

einer Einrichtung zum Anzeigen eines von der Analyseinrichtung gewonnenen Analyseergebnisses, dadurch gekennzeichnet, daß die Schnittstelleneinrichtung (84, 94) weiterhin eine Eingabeeinrichtung zum Eingeben der Attributbilddaten des medizinischen Bilds in Form von digitalen Daten umfaßt, und

daß die Analyseinrichtung eine Einrichtung (92) zum Speichern von Attributdaten, die den Typ des medizinischen Bilds definieren, das durch den computerunterstützten Diagnosealgorithmus analysiert werden kann, und zwar für jeden aus der Mehrzahl von computerunterstützten Diagnosealgorithmen; und eine Einrichtung (88) zum Auswählen eines optimalen computerunterstützten Diagnosealgorithmus, der zum Analysieren des medizinischen Bilds geeignet ist, auf der Basis der in der Speichereinrichtung gespeicherten Attributdaten und der Attributbilddaten des medizinischen, zu analysierenden Bilds; wobei die Analyseinrichtung die medizinischen Bilddaten unter Verwendung des optimalen computerunterstützten Diagnosealgorithmus analysiert, der durch die Wähleinrichtung ausgewählt worden ist.

2. System nach Anspruch 1, dadurch gekennzeichnet, daß es weiterhin aufweist: ein Netzwerk (16) das mit der Schnittstelle verbunden ist;

eine Datenbankeinrichtung (12), die mit dem

Netzwerk verbunden ist und zum Speichern der medizinischen Bilddaten, von von der Analy-
siereinrichtung gebildeten Analyseergebnisda-
ten, und von Assoziationsdaten dient, die die
Beziehung zwischen den medizinischen Bild-
daten und den Analyseergebnisdaten ange-
ben; und

eine Einrichtung zum Einschreiben der Analy-
seergebnisdaten und der Assoziationsdaten in
die Datenbankeinrichtung über das Netzwerk
mit Hilfe der Schnittstelleneinrichtung.

3. System nach Anspruch 1 oder 2, dadurch gekenn-
zeichnet, daß eine Mehrzahl von Modalitäten mit
dem Netzwerk verbunden sind. 15
4. System nach Anspruch 2, dadurch gekennzeichnet,
daß es weiterhin eine Einrichtung (80) zum Eing-
eben von Wiedergewinnungsdaten für die Wiederge-
winning von gewünschten Analyseergebnisdaten,
die in der Datenbankeinrichtung (12) gespeichert
sind; und eine Einrichtung zum Auslesen der Ana-
lyseergebnisdaten aus der Datenbankeinrichtung
(12) in Abhängigkeit von den Wiedergewinnungs-
daten enthält. 20 25
5. System nach Anspruch 1 oder 2, bei dem die Attri-
butbilddaten weiterhin Informationen umfassen, die
angeben, ob ein medizinisches Bild durch einen
Arzt betrachtet worden ist oder nicht, dadurch ge-
kennzeichnet, daß es weiterhin eine Einrichtung
zum selektiven Herausgreifen eines aus einer er-
sten Mehrzahl von medizinischen Bildern, die von
einem Arzt betrachtet worden sind, und/oder eines
aus einer zweiten Mehrzahl von medizinischen Bil-
dern aufweist, die nicht durch einen Arzt betrachtet
worden sind, wobei das Herausgreifen aus der Bas-
is der Attributbilddaten erfolgt, sowie dadurch ge-
kennzeichnet, daß die Analyseinrichtung die me-
dizinischen Bilder, die durch die Einrichtung zum
Herausgreifen herausgegriffen worden sind, unter
Verwendung des optimalen, ausgewählten, compu-
terunterstützten Diagnosealgorithmus analysiert. 30 35 40
6. System nach Anspruch 2, dadurch gekennzeichnet, 45
daß die Attributdaten weiterhin Informationen um-
fassen, die angeben, ob das medizinische Bild
durch die Analyseinrichtung analysiert worden ist
oder nicht. 50
7. System nach Anspruch 6, dadurch gekennzeichnet,
daß die Analyseinrichtung ein medizinisches Bild
analysiert, das durch einen Arzt betrachtet worden
ist, jedoch noch nicht durch die Analyseinrich-
tung analysiert worden ist. 55
8. System nach einem der Ansprüche 5 bis 7, dadurch
gekennzeichnet, daß es weiterhin eine Anzeigeein-

richtung (82, 100, 102) zum Anzeigen des medizi-
nischen Bilds, das noch nicht durch einen Arzt be-
trachtet worden ist, ohne das Analyseergebnis der
Analyseinrichtung, und zum Anzeigen eines me-
dizinischen Bilds, das von einem Arzt betrachtet
worden ist, zusammen mit dem Analyseergebnis
aufweist.

10 Revendications

1. Système pour analyser une image médicale (14) en
utilisant un algorithme de diagnostic assisté par or-
dinateur, comprenant :

des moyens formant interface (84, 94) pour
fournir une image médicale sous forme de don-
nées numériques ;

des moyens de stockage (86) pour stocker les-
dites données d'image médicale, lesdites don-
nées d'image médicale comprenant des don-
nées d'attribut d'image comprenant des infor-
mations concernant le type des images médi-
cales qui peuvent être analysées par des algo-
rithmes de diagnostic assistés par ordinateur ;

des moyens de stockage d'algorithmes (92)
pour stocker une pluralité desdits algorithmes
de diagnostic assistés par ordinateur et desti-
nés à détecter des types différents de parties
anormales dans l'image médicale ;

des moyens d'analyse (88) pour analyser les
données d'image médicale en utilisant l'un des-
dits algorithmes de diagnostic parmi la pluralité
d'algorithmes de diagnostic assistés par ordi-
nateur afin de détecter des parties anormales
dans ladite image médicale ; et

des moyens pour afficher un résultat d'analyse
desdits moyens d'analyse,

caractérisé en ce que

lesdits moyens formant interface (84, 94) com-
prennent en outre des moyens pour entrer les-
dites données d'attribut d'image de l'image mé-
dicale sous forme de données numériques ;

lesdits moyens d'analyse comprennent :

- des moyens (92) pour stocker, pour chacun
desdits algorithmes de diagnostic parmi ladite
pluralité d'algorithmes de diagnostic assistés
par ordinateur, des données d'attribut définis-
sant le type d'images médicales qui peuvent
être analysées par l'algorithme de diagnostic

assisté par ordinateur ;

- des moyens de sélection (88) pour choisir, en se basant sur lesdites données d'attribut stockées dans lesdits moyens de stockage et sur lesdites données d'attribut d'image de l'image médicale à analyser, l'algorithme de diagnostic assisté par ordinateur optimum qui convient pour l'analyse de ladite image médicale, dans lequel

lesdits moyens d'analyse analysent lesdites données d'image médicale en utilisant ledit algorithme de diagnostic assisté par ordinateur optimum choisi par lesdits moyens de sélection.

2. Système selon l'une de la revendication 1, caractérisé en ce qu'il comprend en outre :

un réseau (16) connecté auxdits moyens formant interface ;

une base de données (12) connectée audit réseau et destinée à stocker les données d'images médicales, ainsi que des données de résultats d'analyses desdits moyens d'analyse et des données d'association indiquant la relation entre les données d'images médicales et les données de résultats d'analyses ; et

des moyens d'écriture, pour écrire lesdites données de résultats d'analyses et lesdites données d'association dans ladite base de données via ledit réseau à l'aide desdits moyens formant interface.

3. Système selon l'une ou l'autre des revendications 1 et 2, caractérisé en ce qu'une pluralité de modalités sont connectées audit réseau.

4. Système selon la revendication 2, caractérisé en ce qu'il comprend en outre :

des moyens d'entrée (80) pour entrer des données de recherche afin de rechercher des données de résultats d'analyses désirées stockées dans ladite base de données (12) ; et

des moyens de lecture pour lire les données de résultats d'analyses depuis ladite base de données (12) en accord avec lesdites données de recherche.

5. Système selon l'une ou l'autre des revendications 1 et 2, dans lequel lesdites données d'attributs d'images comprennent en outre des informations indiquant si une image médicale a été ou non revue par un médecin, caractérisé en ce qu'il comprend

en outre :

des moyens pour extraire sélectivement une image médicale d'une première pluralité d'images médicales qui ont été revues par un médecin, et une image médicale parmi une deuxième pluralité d'images médicales qui n'ont pas été revues par un médecin, en se basant sur lesdites données d'attributs d'images, et caractérisé en ce que lesdits moyens d'analyse analysent lesdites images médicales extraites par lesdits moyens d'extraction en utilisant ledit algorithme de diagnostic optimum choisi parmi ladite pluralité d'algorithmes de diagnostic assistés par ordinateur.

6. Système selon la revendication 2, caractérisé en ce que lesdites données d'attributs d'images comprennent en outre des informations indiquant si l'image médicale a été analysée ou non par lesdits moyens d'analyse.

7. Système selon la revendication 6, caractérisé en ce que lesdits moyens d'analyse analysent une image médicale qui a été revue par un médecin mais qui n'a pas été analysée par lesdits moyens d'analyse.

8. Système selon l'une quelconque des revendications 5 à 7, caractérisée en ce qu'il comprend en outre des moyens d'affichage (82, 100, 102) pour afficher l'image médicale qui n'a pas été revue par un médecin, sans les résultats d'analyses desdits moyens d'analyse, et pour afficher l'image médicale qui a été revue par un médecin, avec les résultats d'analyses.

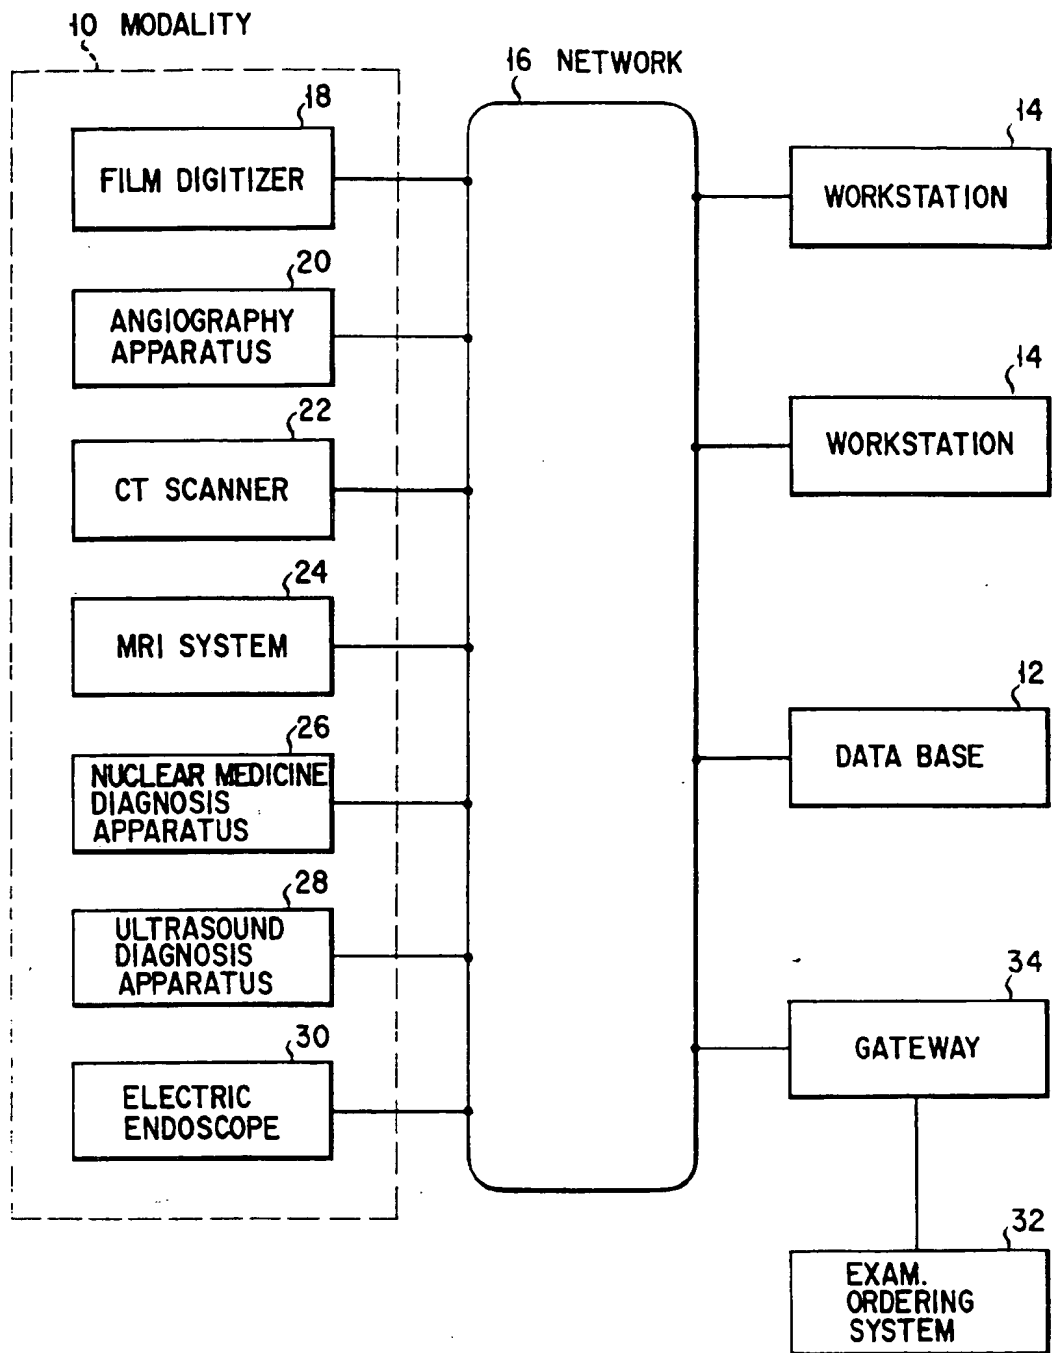


FIG. 1

EXAMINATION DATA
EXAM. ID NUMBER
PATIENT ID NUMBER
NAME OF PATIENT
BIRTHDAY
SEX DISTINCTION
MODALITY
OBJECT
DATE
EXAM. REQUESTING DEPARTMENT
NAME OF DOCTOR
THE NUMBER OF IMAGES

FIG. 2

EXAM. DATA(X-RAY RADIOGRAPH OF CHEST)	
EXAM. ID	K3-905-002-005
PATIENT ID	N-T-239650
NAME
BIRTHDAY	'55-4-5
SEX	MALE
MODALITY	CONVENTIONAL RADIOGRAPH
OBJECT	CHEST
DATE	'90-3-3
DEPARTMENT	SURGERY
DOCTOR
THE NUMBER OF IMAGES	4
.	

FIG. 3

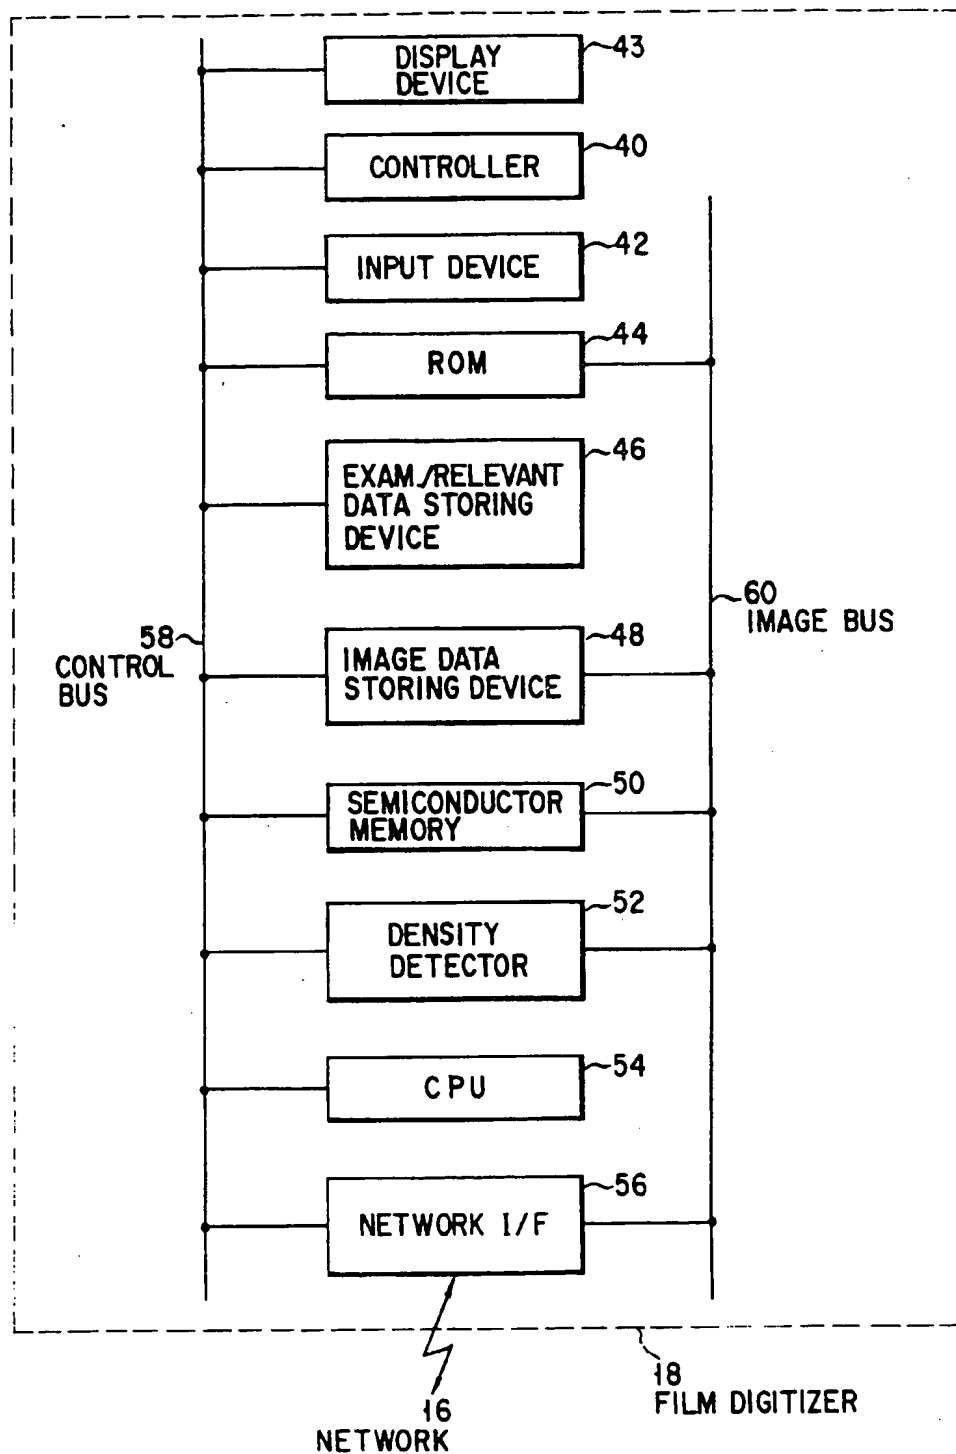


FIG. 4

RELEVANT DATA
EXAM. ID
IMAGE ID
SIZE OF IMAGE (WIDTH)
SIZE OF IMAGE (LENGTH)
MATRIX SIZE (WIDTH)
MATRIX SIZE (LENGTH)
BIT LENGTH OF PIXEL DATA
AMOUNT OF IMAGE DATA
RESULT OF CAD ID ₁ ADDRESS 1
RESULT OF CAD ID ₂ ADDRESS 2
⋮
RESULT OF CAD ID _n ADDRESS _n
THE NUMBER OF APPLICATIONS OF CAD ALGORITHM
IMAGING DIRECTION
READING

FIG. 5

RELEVANT DATA	
EXAM. ID	K3-905-002-005
IMAGE ID	2
SIZE OF IMAGE (WIDTH)	500
SIZE OF IMAGE (LENGTH)	500
MATRIX SIZE (WIDTH)	1024
MATRIX SIZE (LENGTH)	1024
BIT LENGTH OF PIXEL DATA	10
AMOUNT OF IMAGE DATA (MB)	5
RESULT OF CAD ID1 ADDRESS 1	A1111
RESULT OF CAD ID2 ADDRESS 2	NOTHING
⋮	⋮
RESULT OF CAD IDn ADDRESS n	NOTHING
THE NUMBER OF APPLICATIONS OF CAD ALGORITHM	0
IMAGING DIRECTION	FRONT
READING	NOTHING

FIG. 6

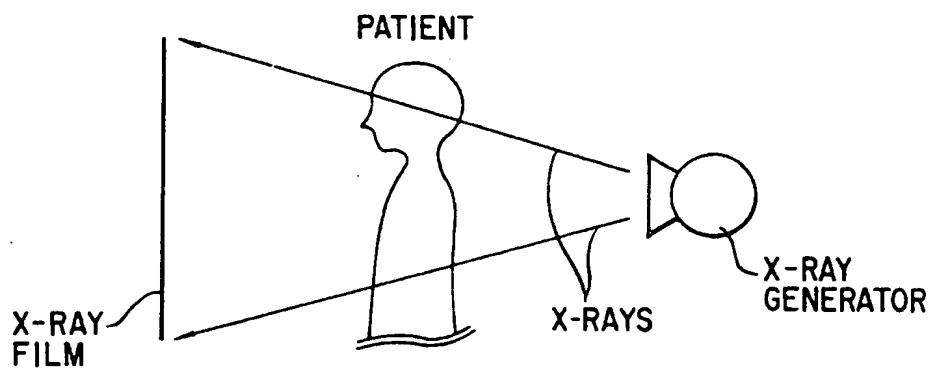


FIG. 7

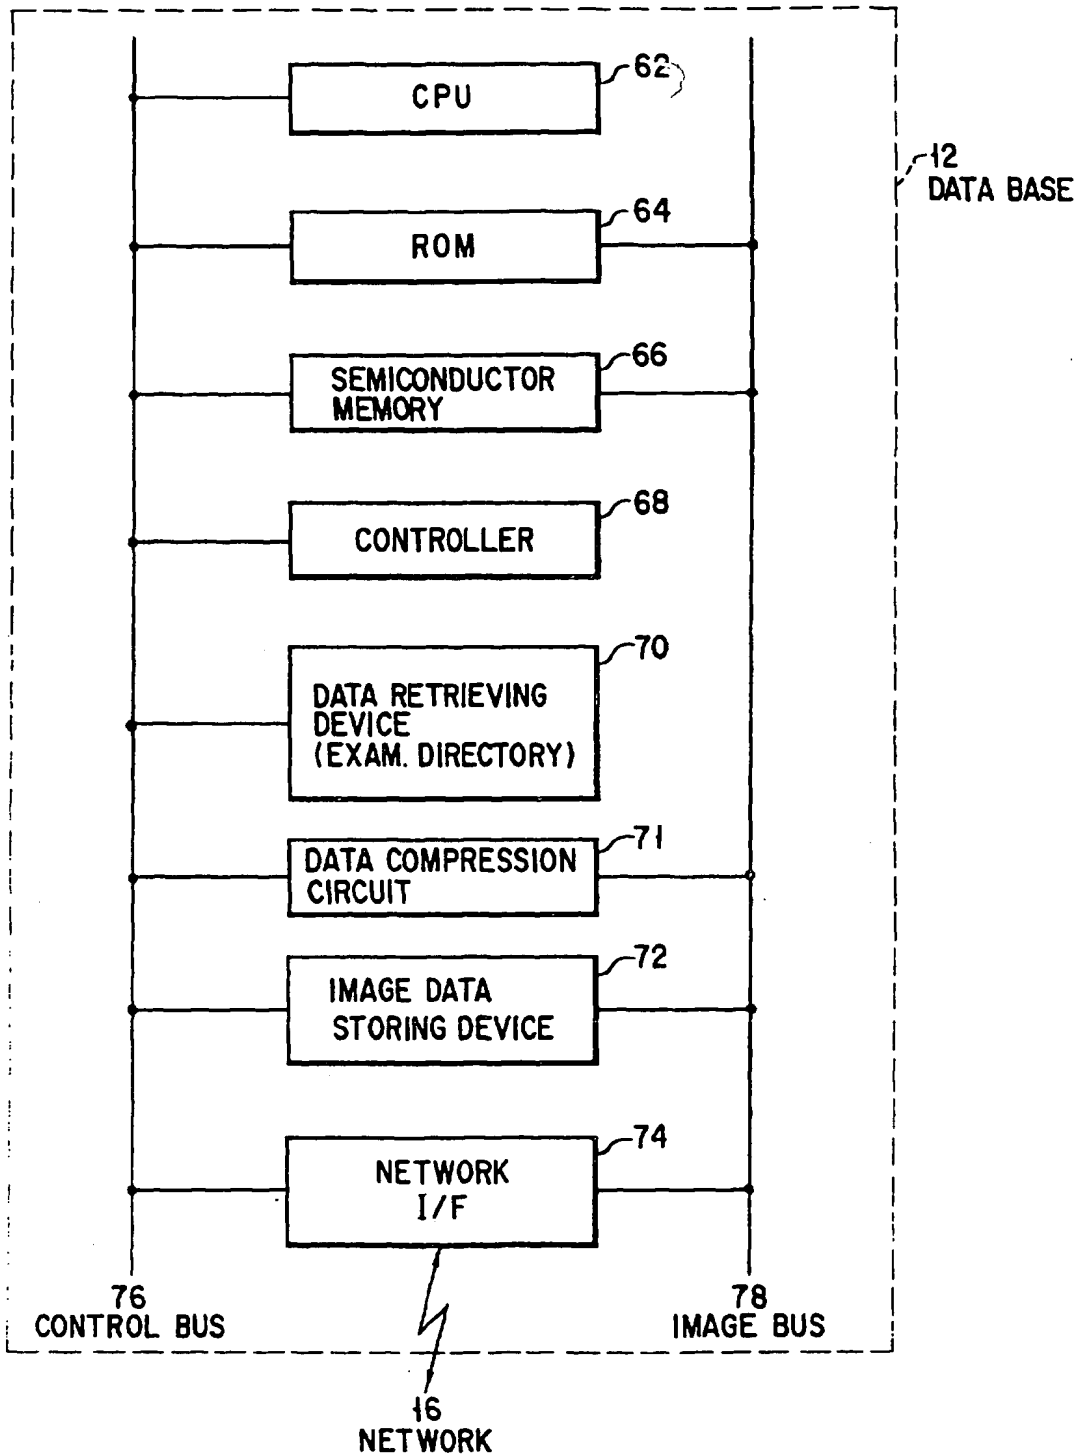


FIG. 8

EXAM. DIRECTORY	
EXAM. ID	EXAM. DATA
PATIENT ID	
NAME OF PATIENT	
BIRTHDAY	
SEX	
MODALITY	
EXAM. OBJECT	
EXAM. DATE	
EXAM. DEPARTMENT	
EXAM. REQUESTING DOCTOR	
THE NUMBER OF IMAGES	
:	
ADDRESS OF READING REPORT	
AMOUNT OF REPORT DATA	FIRST IMAGE
ADDRESS OF RELEVANT DATA	
AMOUNT OF RELEVANT DATA	
ADDRESS OF IMAGE DATA	
AMOUNT OF IMAGE DATA	
RESULT OF CAD ID ₁ ADDRESS 1	
:	N-th IMAGE
RESULT OF CAD ID _n ADDRESS n	
:	
ADDRESS OF RELEVANT DATA	N-th IMAGE
AMOUNT OF RELEVANT DATA	
ADDRESS OF IMAGE DATA	
AMOUNT OF IMAGE DATA	
RESULT OF CAD ID ₁ ADDRESS 1	
:	

FIG. 9

DOCTOR ID	REQUESTING DOCTOR ID	MODALITY	OBJECT	EXAM. ID
A3332	B4441	RADIOGRAPH	CHEST	C6661 C6662 . . .
A3333 . . .				

FIG. 10

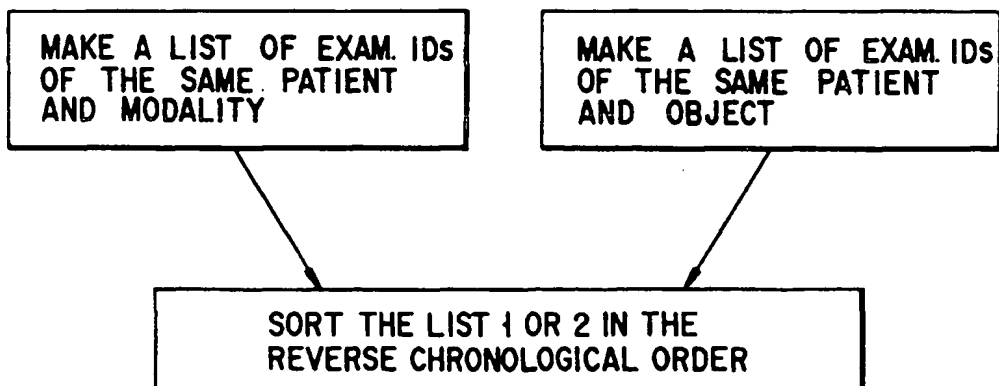


FIG. 11

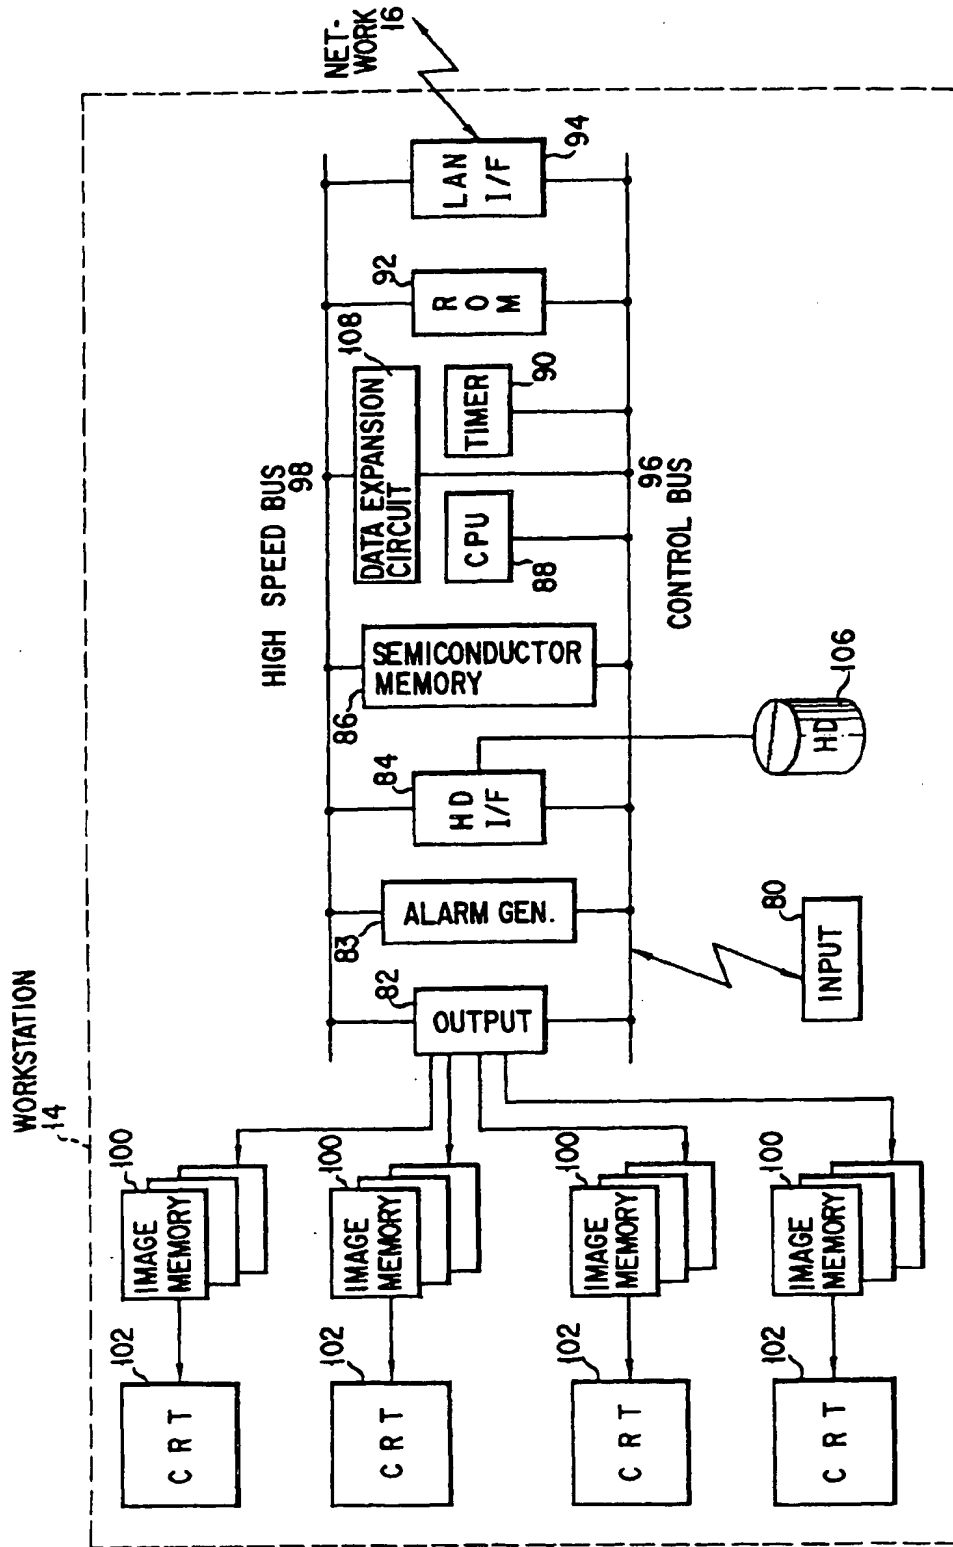


FIG. 12

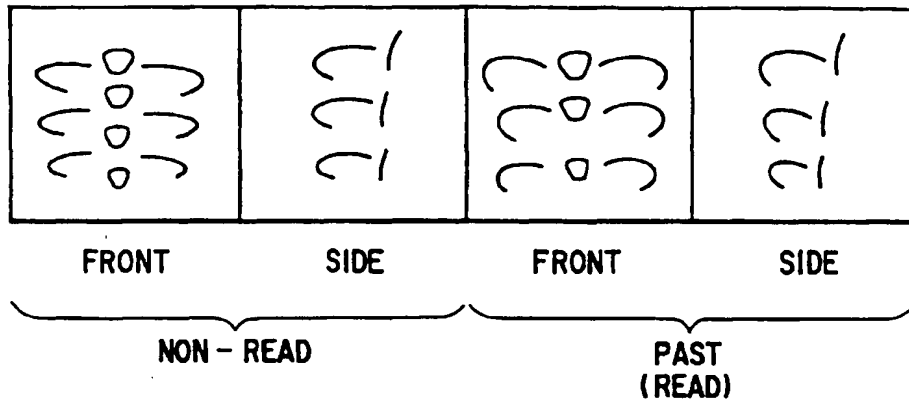


FIG. 13

CRT IMAGE DISPLAY CONTROL TABLE		
CRT ID	EXAM. ID	IMAGE ID
1	K3-905-002-005	1
2	K3-905-002-005	2
3		
4		
⋮	⋮	⋮

FIG. 14

NAME OF CAD ALGORITHM	ATTRIBUTE DATA	
	ITEM	CONTENTS
INTERSTITIAL LUNG DISEASE	MODALITY	CONVENTIONAL RADIOGRAPH
	EXAM. OBJECT	CHEST
	IMAGING DIRECTION	FRONT
	RESULT OF CAD	NOTHING
MICRO CARCIFICATION DETECTION IN MAMMOGRAPHY	MODALITY	MAMMOGRAPH
	EXAM. OBJECT	MAMMA
	IMAGING DIRECTION	LEFT SIDE
	RESULT OF CAD	NOTHING
...		
HEART SIZE	MODALITY	CONVENTIONAL RADIOGRAPH
	EXAM. OBJECT	CHEST
	IMAGING DIRECTION	FRONT
	RESULT OF CAD	NOTHING

FIG. 15

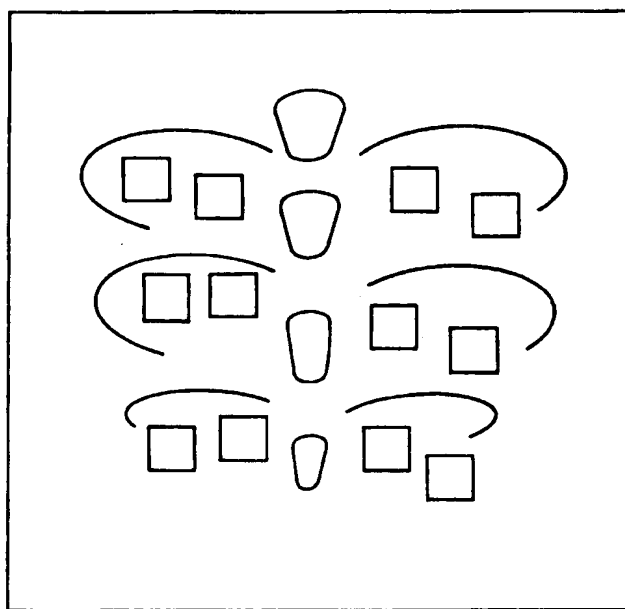


FIG. 16

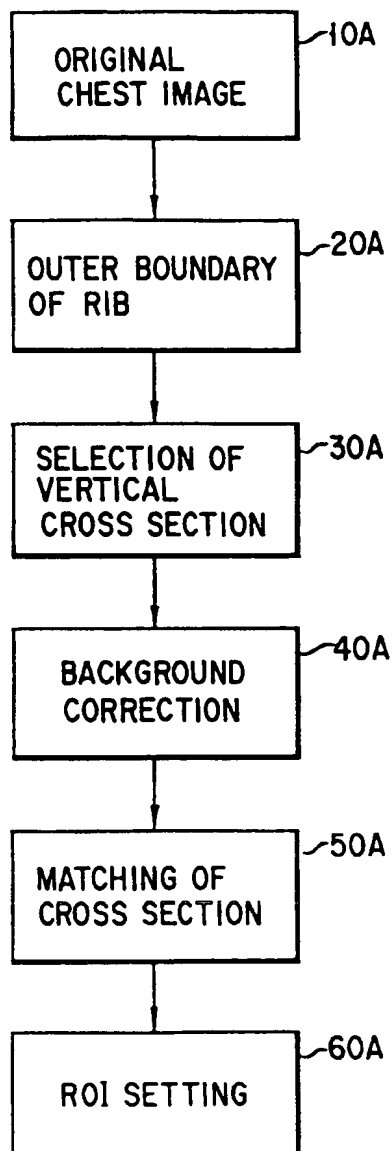


FIG. 17

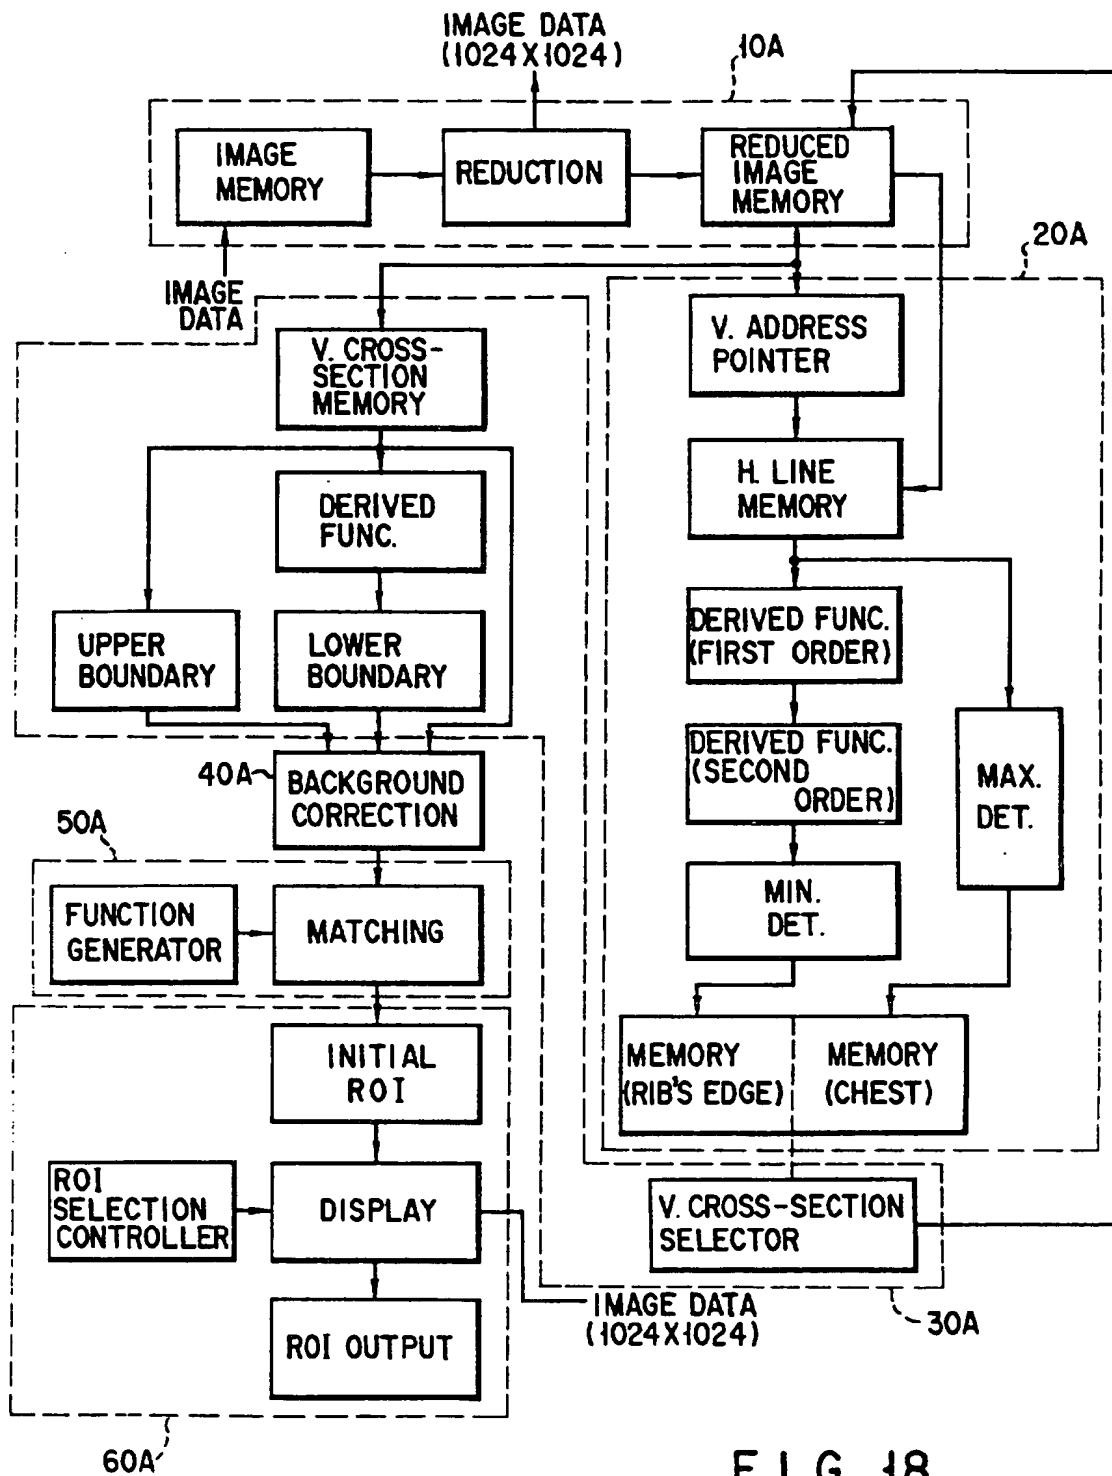


FIG. 18

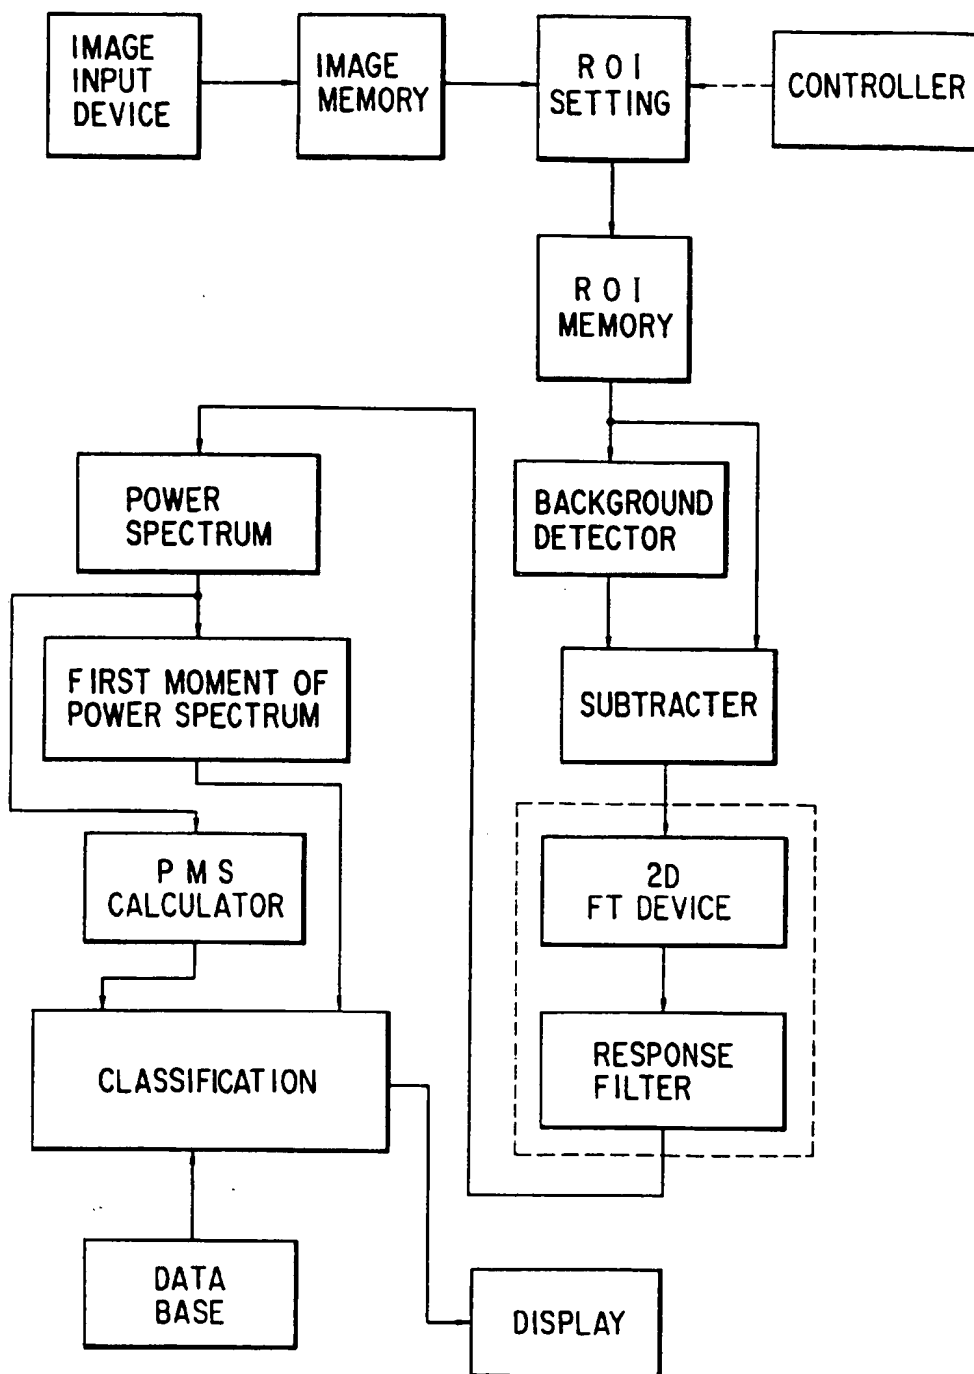


FIG. 19

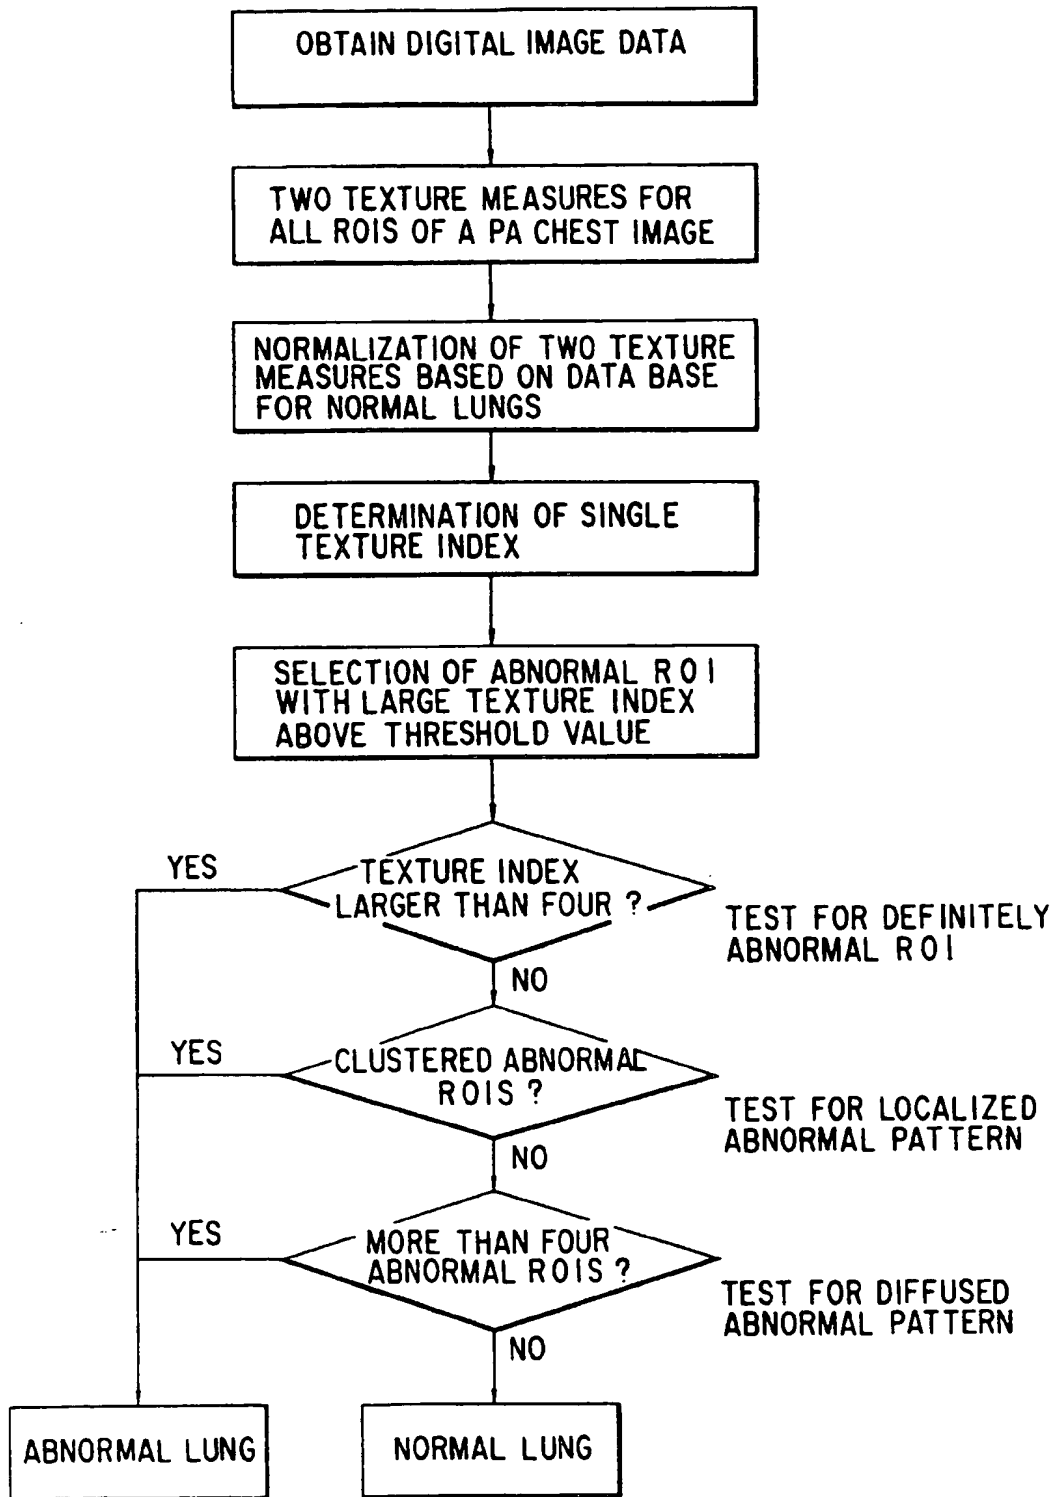


FIG. 20

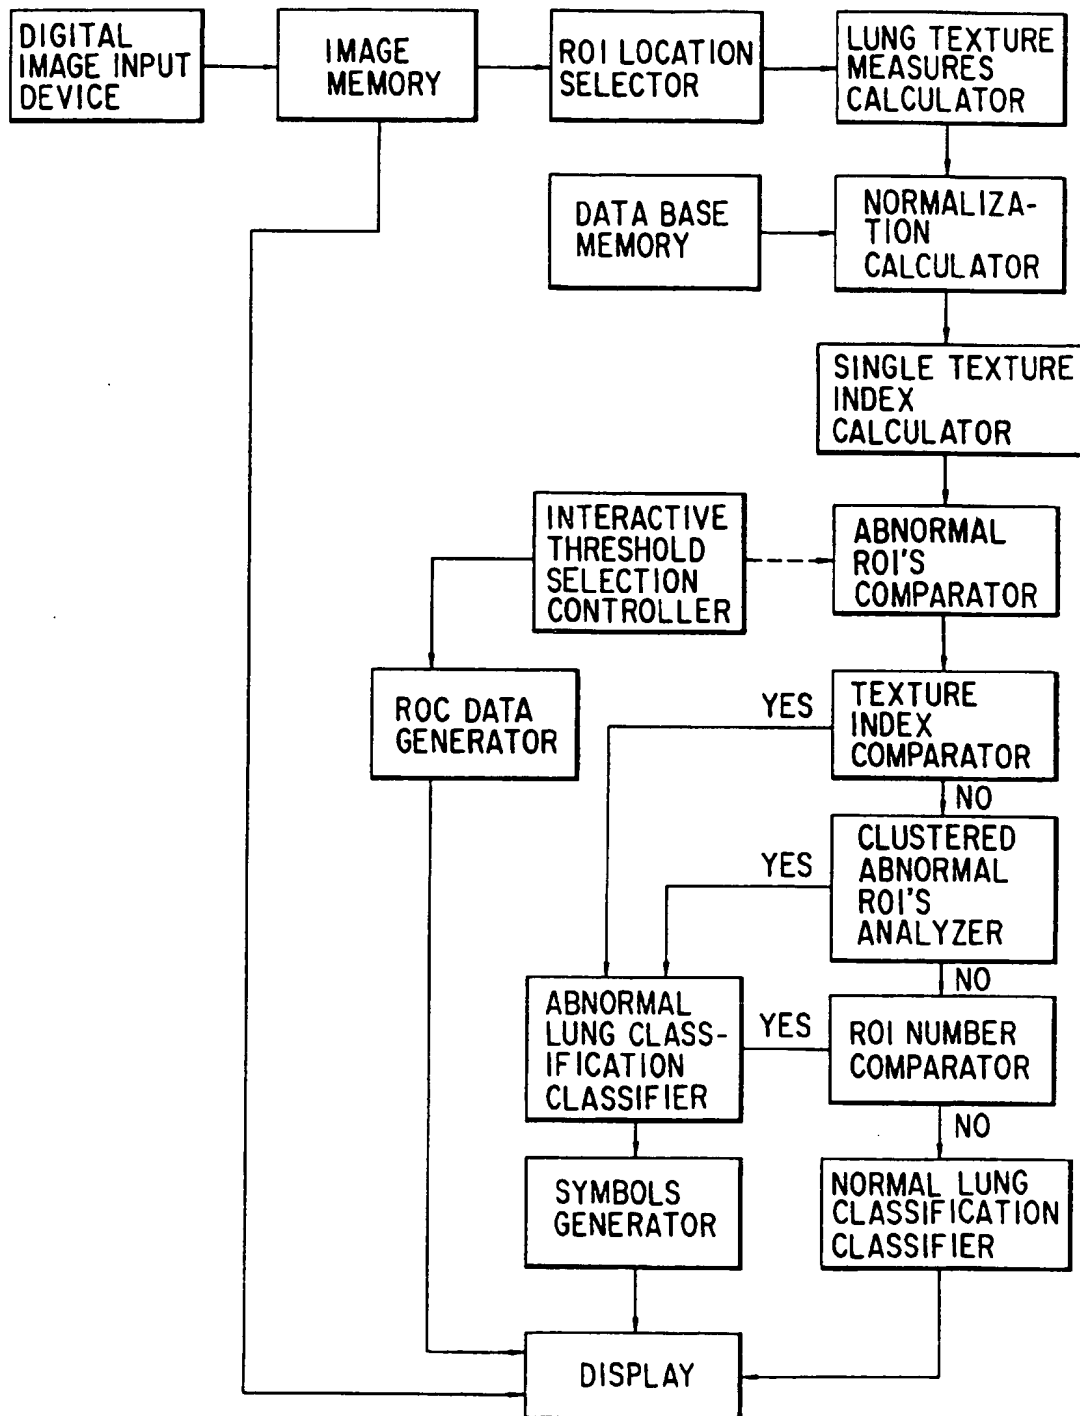


FIG. 21

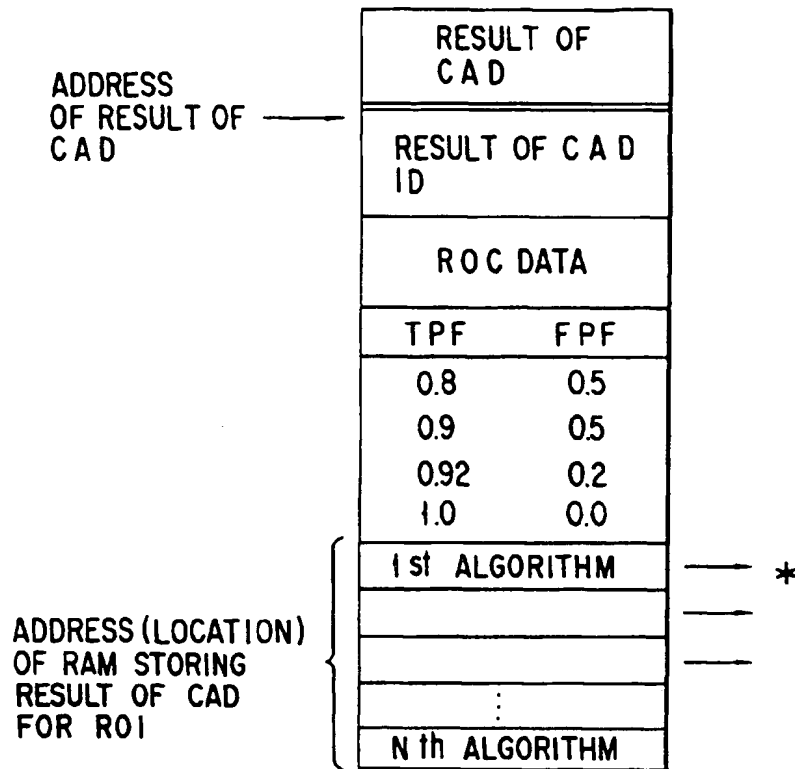
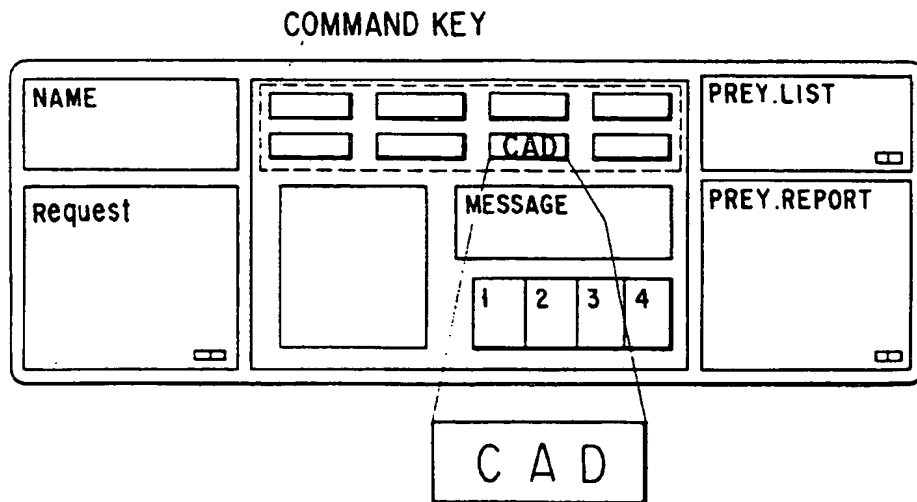
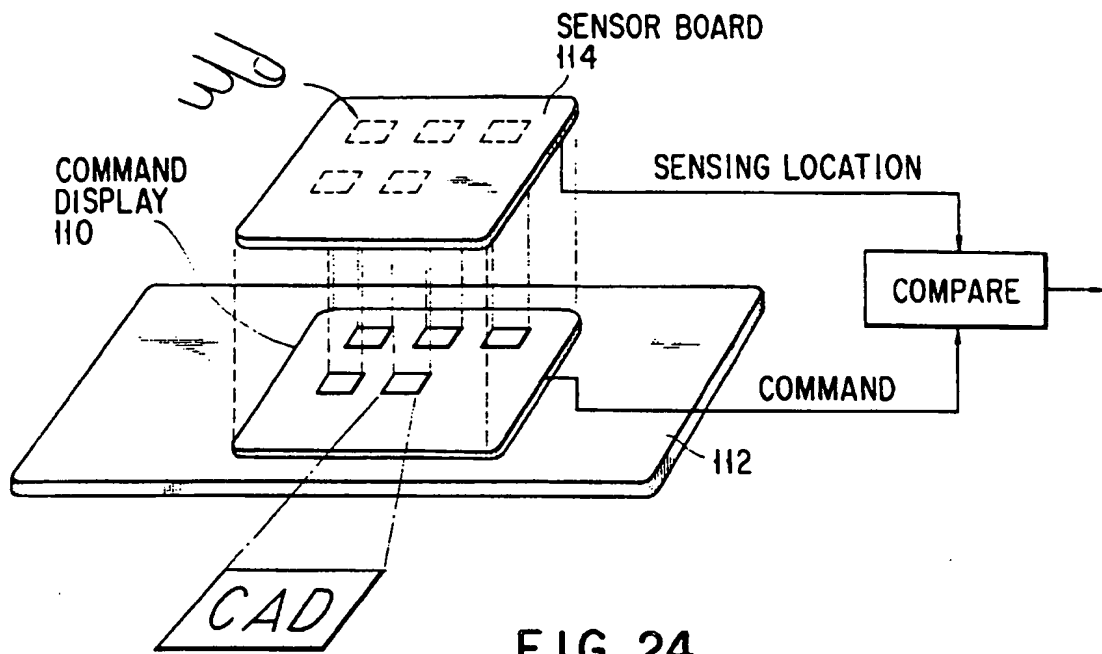


FIG. 22

* —	ROI LOCATION		X	300
			Y	250
	FEATURE	RMS VARIATION		10.5
		FIRST MOMENT		1.8
	NORMAL / ABNORMAL			
TYPE OF ABNORMALITY				NODULAR
PATTERN OF ABNORMALITY				LOCAL

FIG. 23



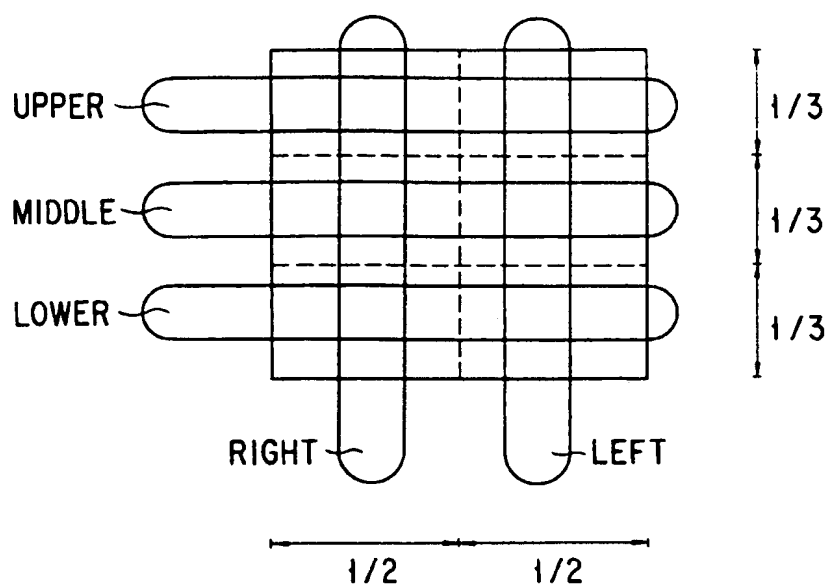


FIG. 26

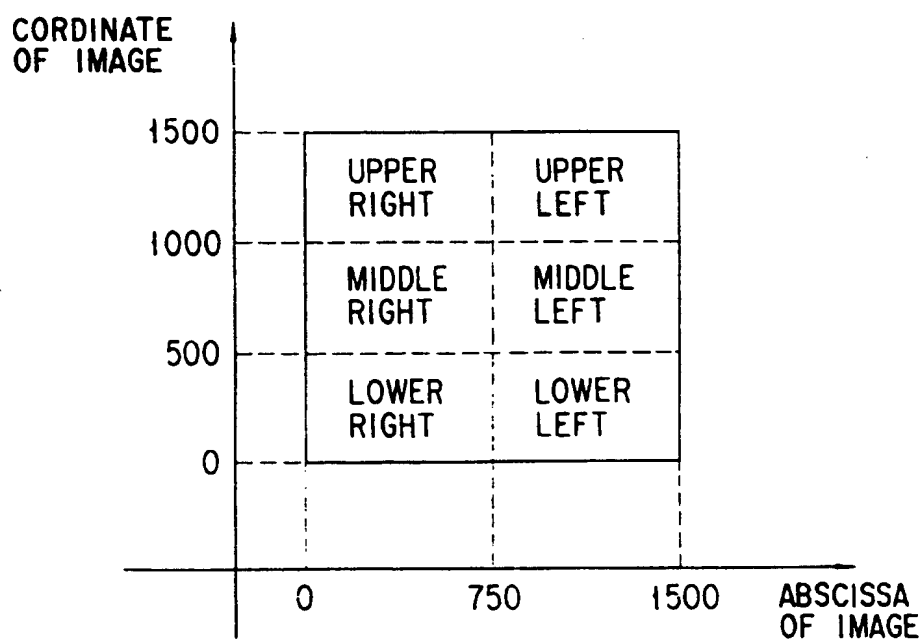


FIG. 27

EXPRESSION OF ABNORMALITY		EXPRESSION OF ABNORMALITY					
	RIGHT		UPPER			UPPER RIGHT	LUNG ABNORMAL
				MIDDLE		MIDDLE RIGHT	
					LOWER	LOWER RIGHT	
		LEFT	UPPER			UPPER LEFT	
				MIDDLE		MIDDLE LEFT	
					LOWER	LOWER LEFT	
EXPRESSION OF ABNORMALITY	RIGHT		LEFT		UPPER		LUNG ABNORMAL
					MIDDLE		
EXPRESSION OF ABNORMALITY	ABNORMAL		ABNORMAL		ABNORMAL		MORE THAN TWO IN RIGHT, LEFT, UPPER, MIDDLE, OR LOWER
	CONDITION OF THE NUMBER OF ABNORMAL ROIS		MORE THAN TWO IN RIGHT, LEFT, UPPER, MIDDLE, OR LOWER		MORE THAN TWO IN UPPER OR LOWER		

FIG. 28

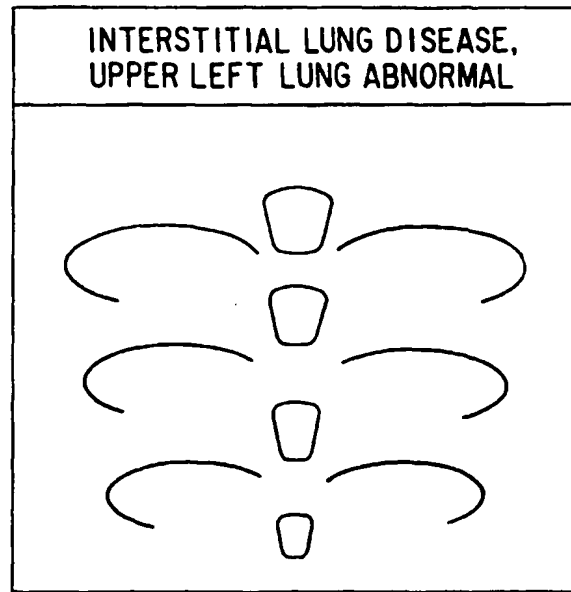


FIG. 29

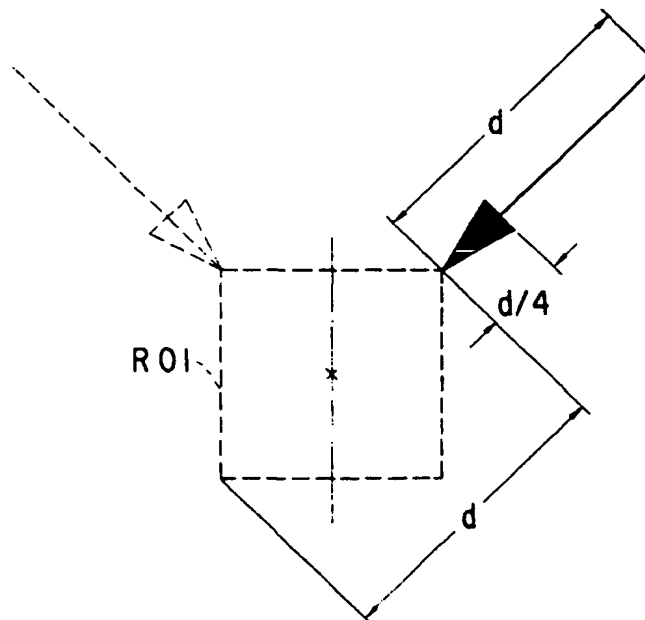


FIG. 30

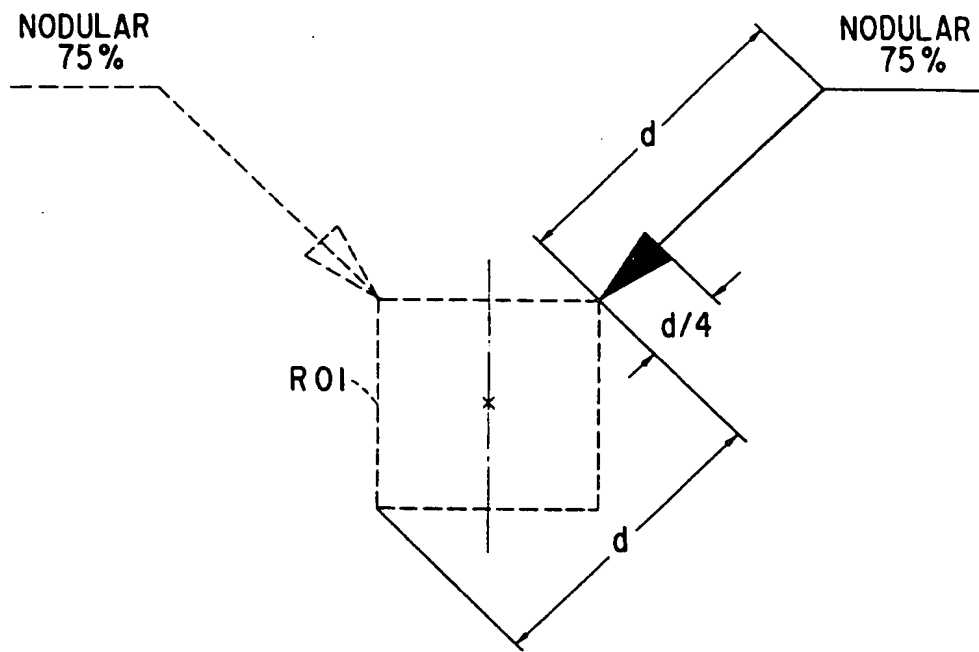


FIG. 31

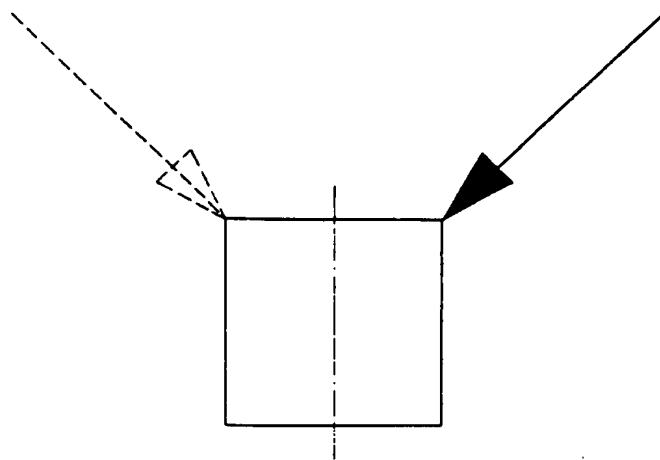


FIG. 32

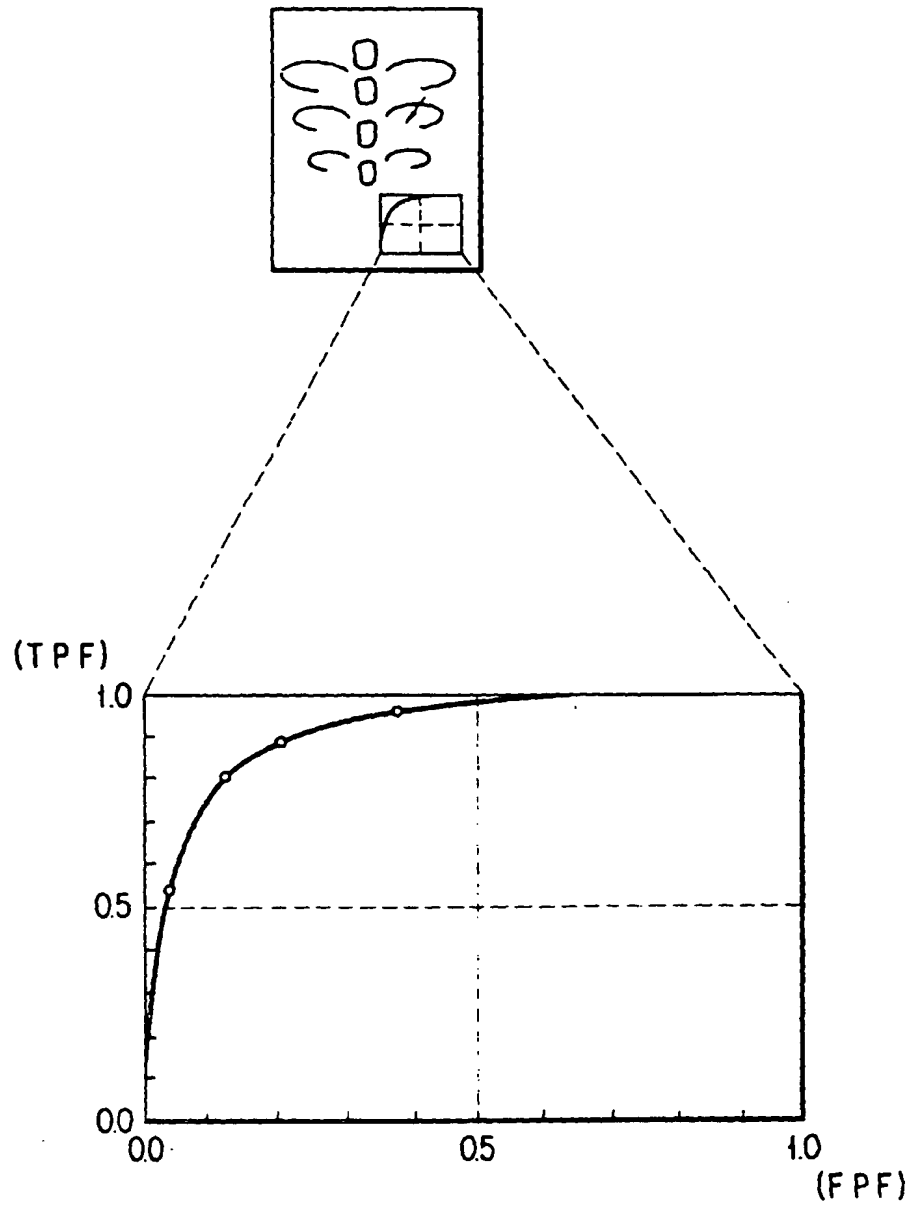


FIG. 33

RELEVANT DATA ⋮
RESULT OF CAD 1
RESULT OF CAD 2
⋮
RESULT OF CAD n

FIG. 34

RELEVANT DATA	⋮
	RESULT OF CAD 1 ID 1 ADDRESS 1 (AAA)
	⋮
	RESULT OF CAD n ID n ADDRESS n
AAA →	
RESULT OF CAD 1	
RESULT OF CAD 2	
⋮	
RESULT OF CAD n	

FIG. 35

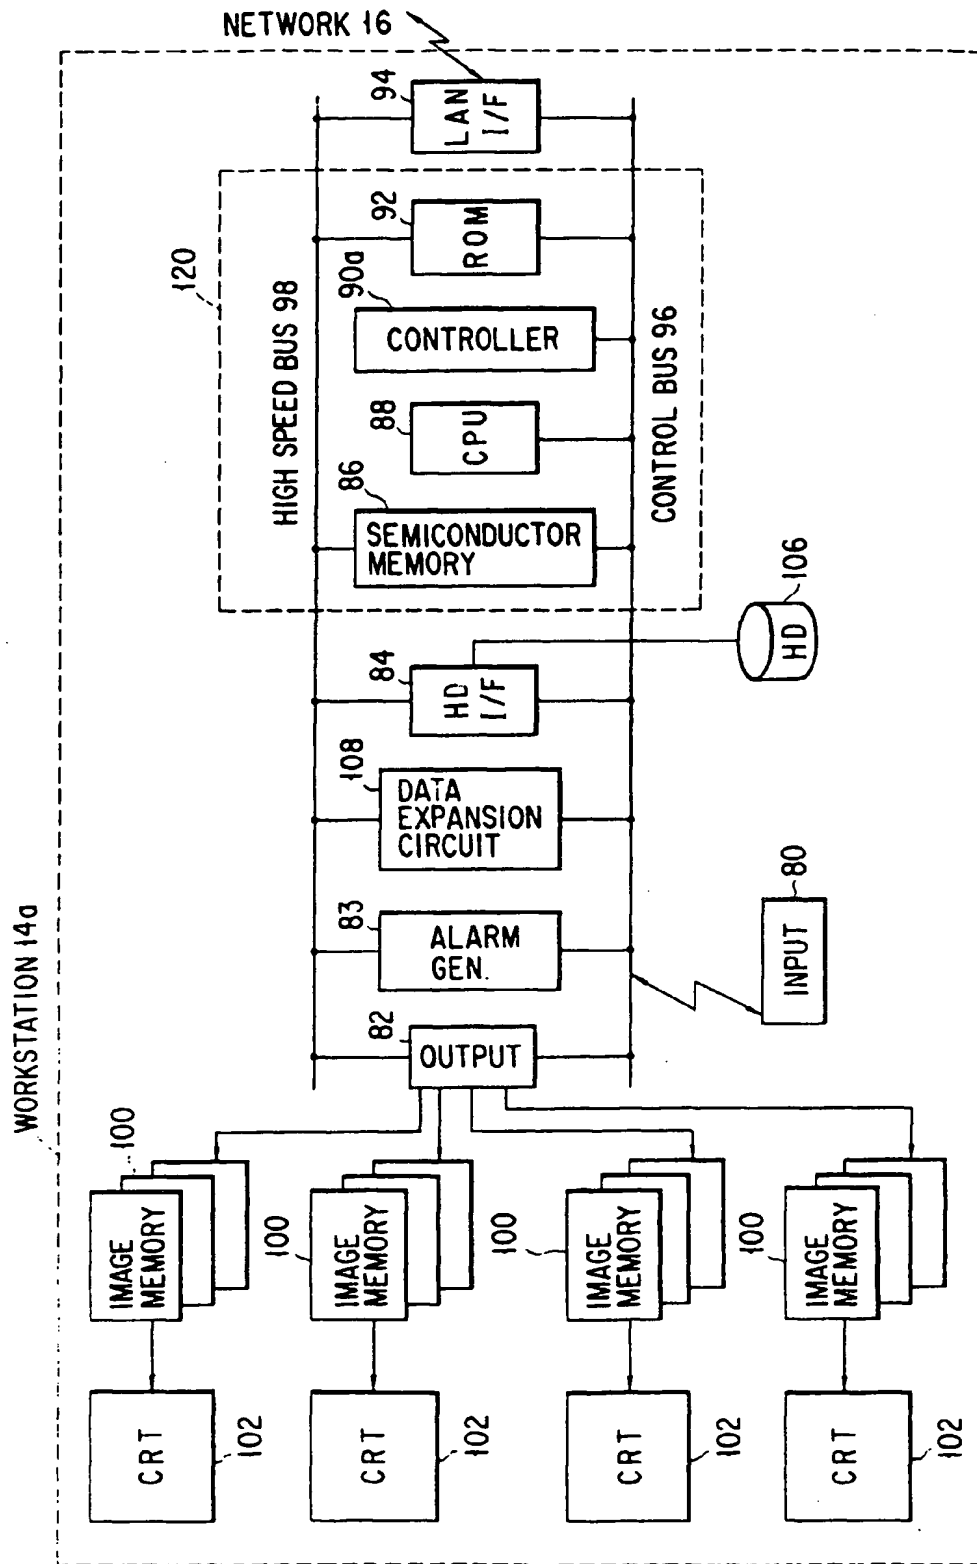


FIG. 36

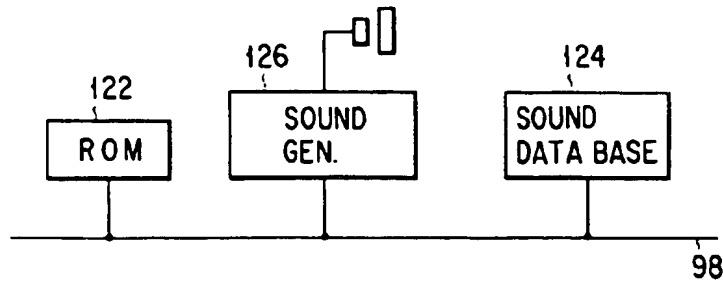


FIG. 37

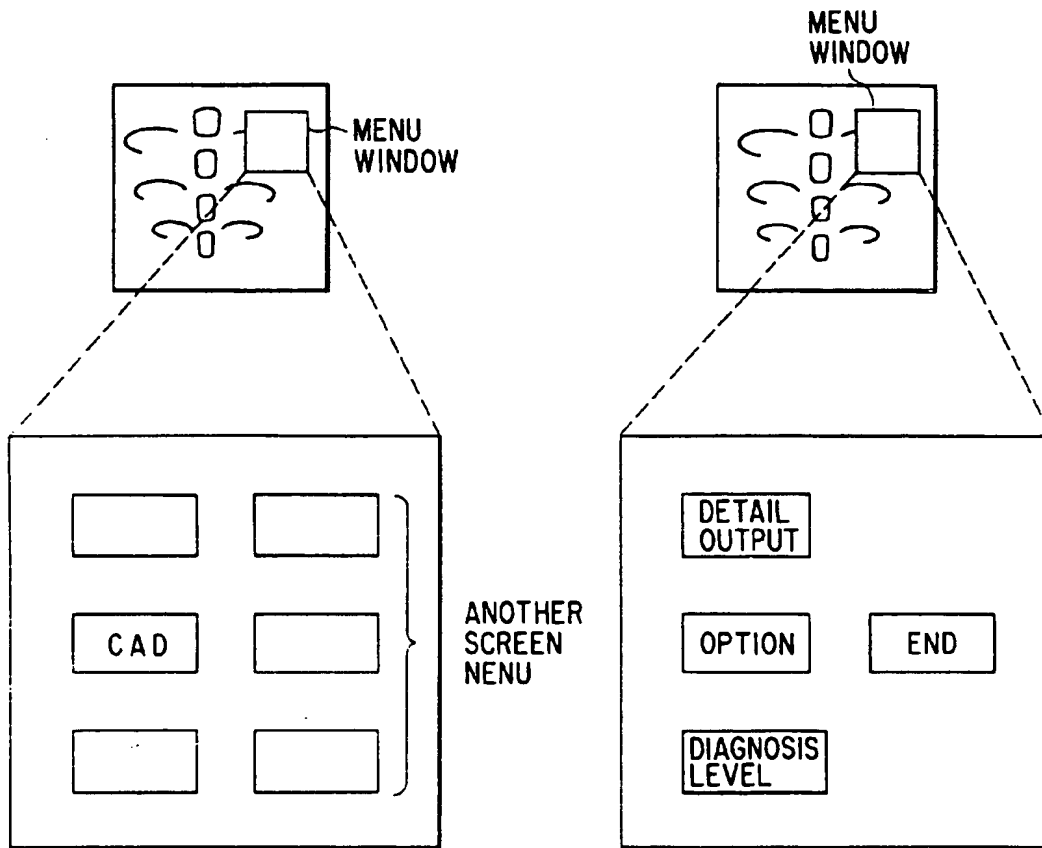


FIG. 38A

FIG. 38B

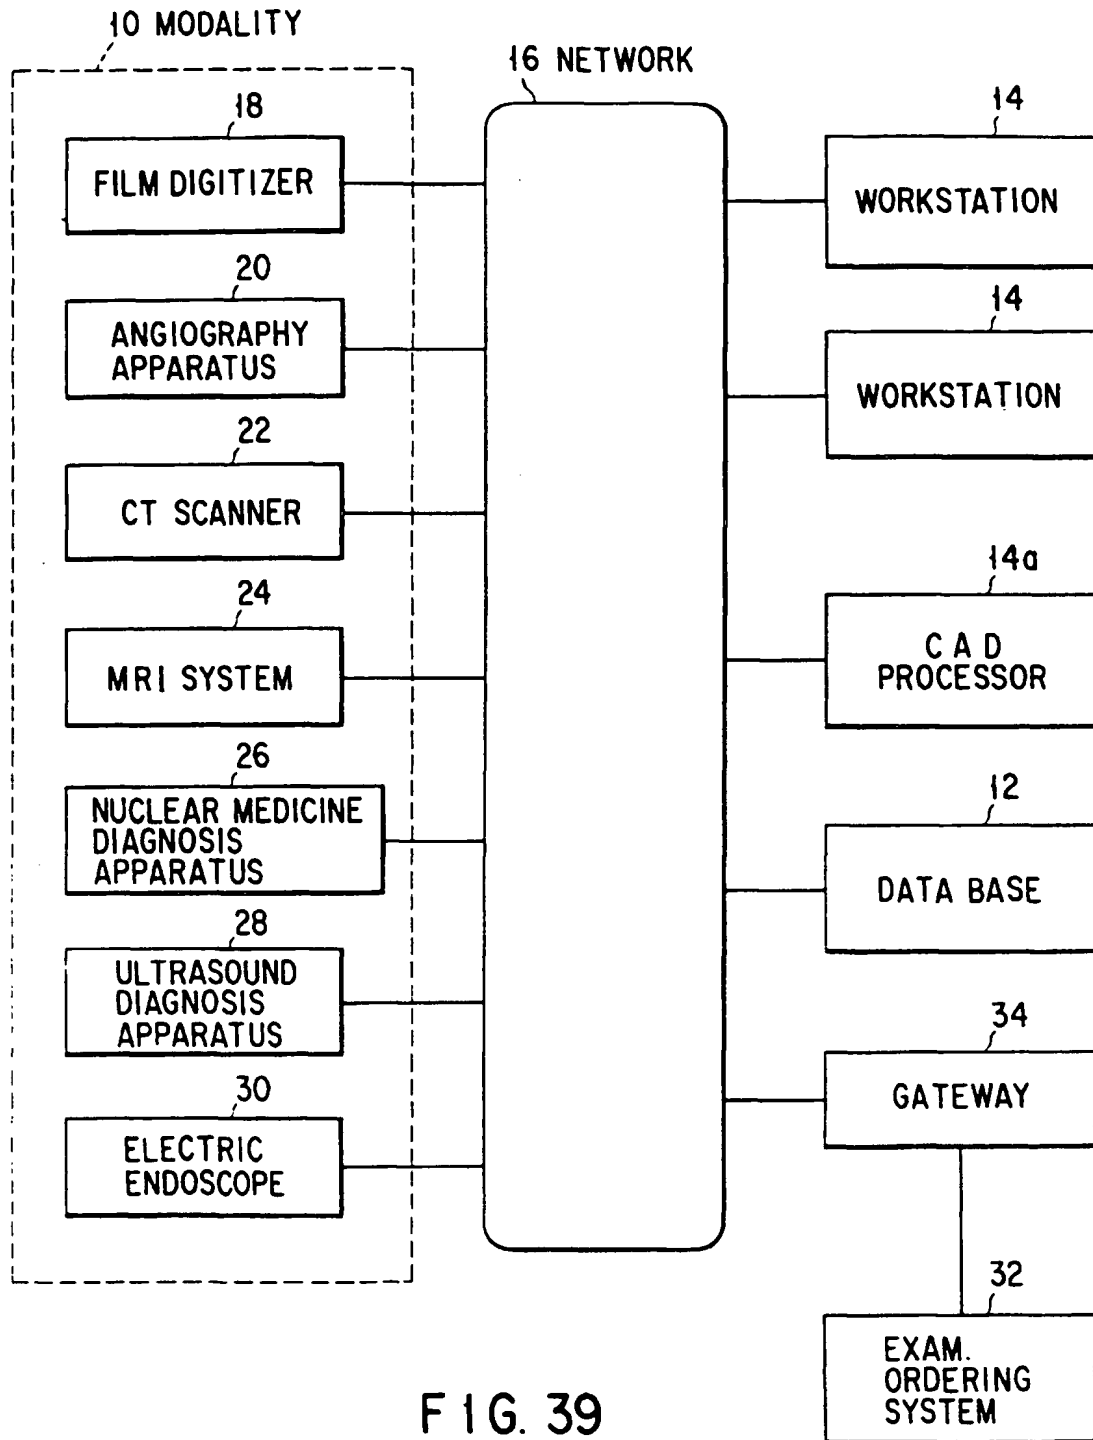


FIG. 39




FIG. 40A




FIG. 40B




FIG. 40C




FIG. 40D




FIG. 40E




FIG. 41A




FIG. 41B




FIG. 41C




FIG. 41D




FIG. 41E




FIG. 41F

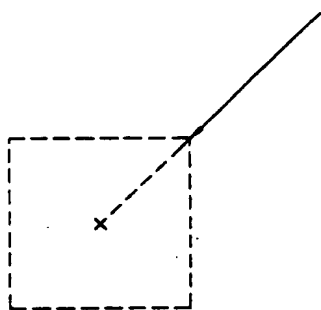


FIG. 42A

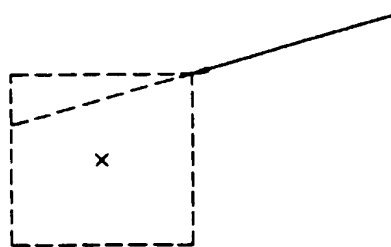


FIG. 42B

INTERSTITIAL LUNG DISEASE DETECTION CAD
LUNG NODULAR SHADOW DETECTION CAD
HEAT SIZE DETECTION CAD

F I G. 43

**This Page is Inserted by IFW Indexing and Scanning
Operations and is not part of the Official Record**

BEST AVAILABLE IMAGES

Defective images within this document are accurate representations of the original documents submitted by the applicant.

Defects in the images include but are not limited to the items checked:

- ☐ **BLACK BORDERS**
- ☐ **IMAGE CUT OFF AT TOP, BOTTOM OR SIDES**
- ☐ **FADED TEXT OR DRAWING**
- ☐ **BLURRED OR ILLEGIBLE TEXT OR DRAWING**
- ☐ **SKEWED/SLANTED IMAGES**
- ☐ **COLOR OR BLACK AND WHITE PHOTOGRAPHS**
- ☐ **GRAY SCALE DOCUMENTS**
- ☐ **LINES OR MARKS ON ORIGINAL DOCUMENT**
- ☒ **REFERENCE(S) OR EXHIBIT(S) SUBMITTED ARE POOR QUALITY**
- ☐ **OTHER:** _____

IMAGES ARE BEST AVAILABLE COPY.

As rescanning these documents will not correct the image problems checked, please do not report these problems to the IFW Image Problem Mailbox.